

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070119\
 Data File : BM021309.D
 Acq On : 01 Jul 2019 15:02
 Operator : HP/JU
 Sample : PB121037BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK37

Quant Time: Jul 02 00:54:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 01 01:16:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	196915	20.00	ng/ul	0.00
18) Naphthalene-d8	10.54	136	872828	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	537457	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1083917	20.00	ng/ul	0.00
77) Chrysene-d12	21.34	240	814129	20.00	ng/ul	0.00
85) Perylene-d12	23.61	264	972254	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	25264	6.09	ng/uL	0.00
5) Phenol-d5	6.93	99	530358	30.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	303743	29.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	446630	32.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	463674	32.41	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	238633	33.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	281782	35.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	530503	33.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	658258	39.45	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	1618025	33.32	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	1955142	32.89	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	168632	21.35	ng/ul	0.00
57) Fluorene-d10	15.39	176	1354562	32.07	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	132219	19.84	ng/ul	0.00
70) Anthracene-d10	17.24	188	1838249	32.63	ng/ul	0.00
78) Pyrene-d10	19.54	212	1657170	33.92	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	1870060	32.60	ng/ul	0.00


Target Compounds					Qvalue	
45) 2,6-Dinitrotoluene	13.82	165	11584	1.373	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070119\
Data File : BM021309.D
Acq On : 01 Jul 2019 15:02
Operator : HP/JU
Sample : PB121037BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK37

Quant Time: Jul 02 00:54:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 01 01:16:07 2019
Response via : Initial Calibration

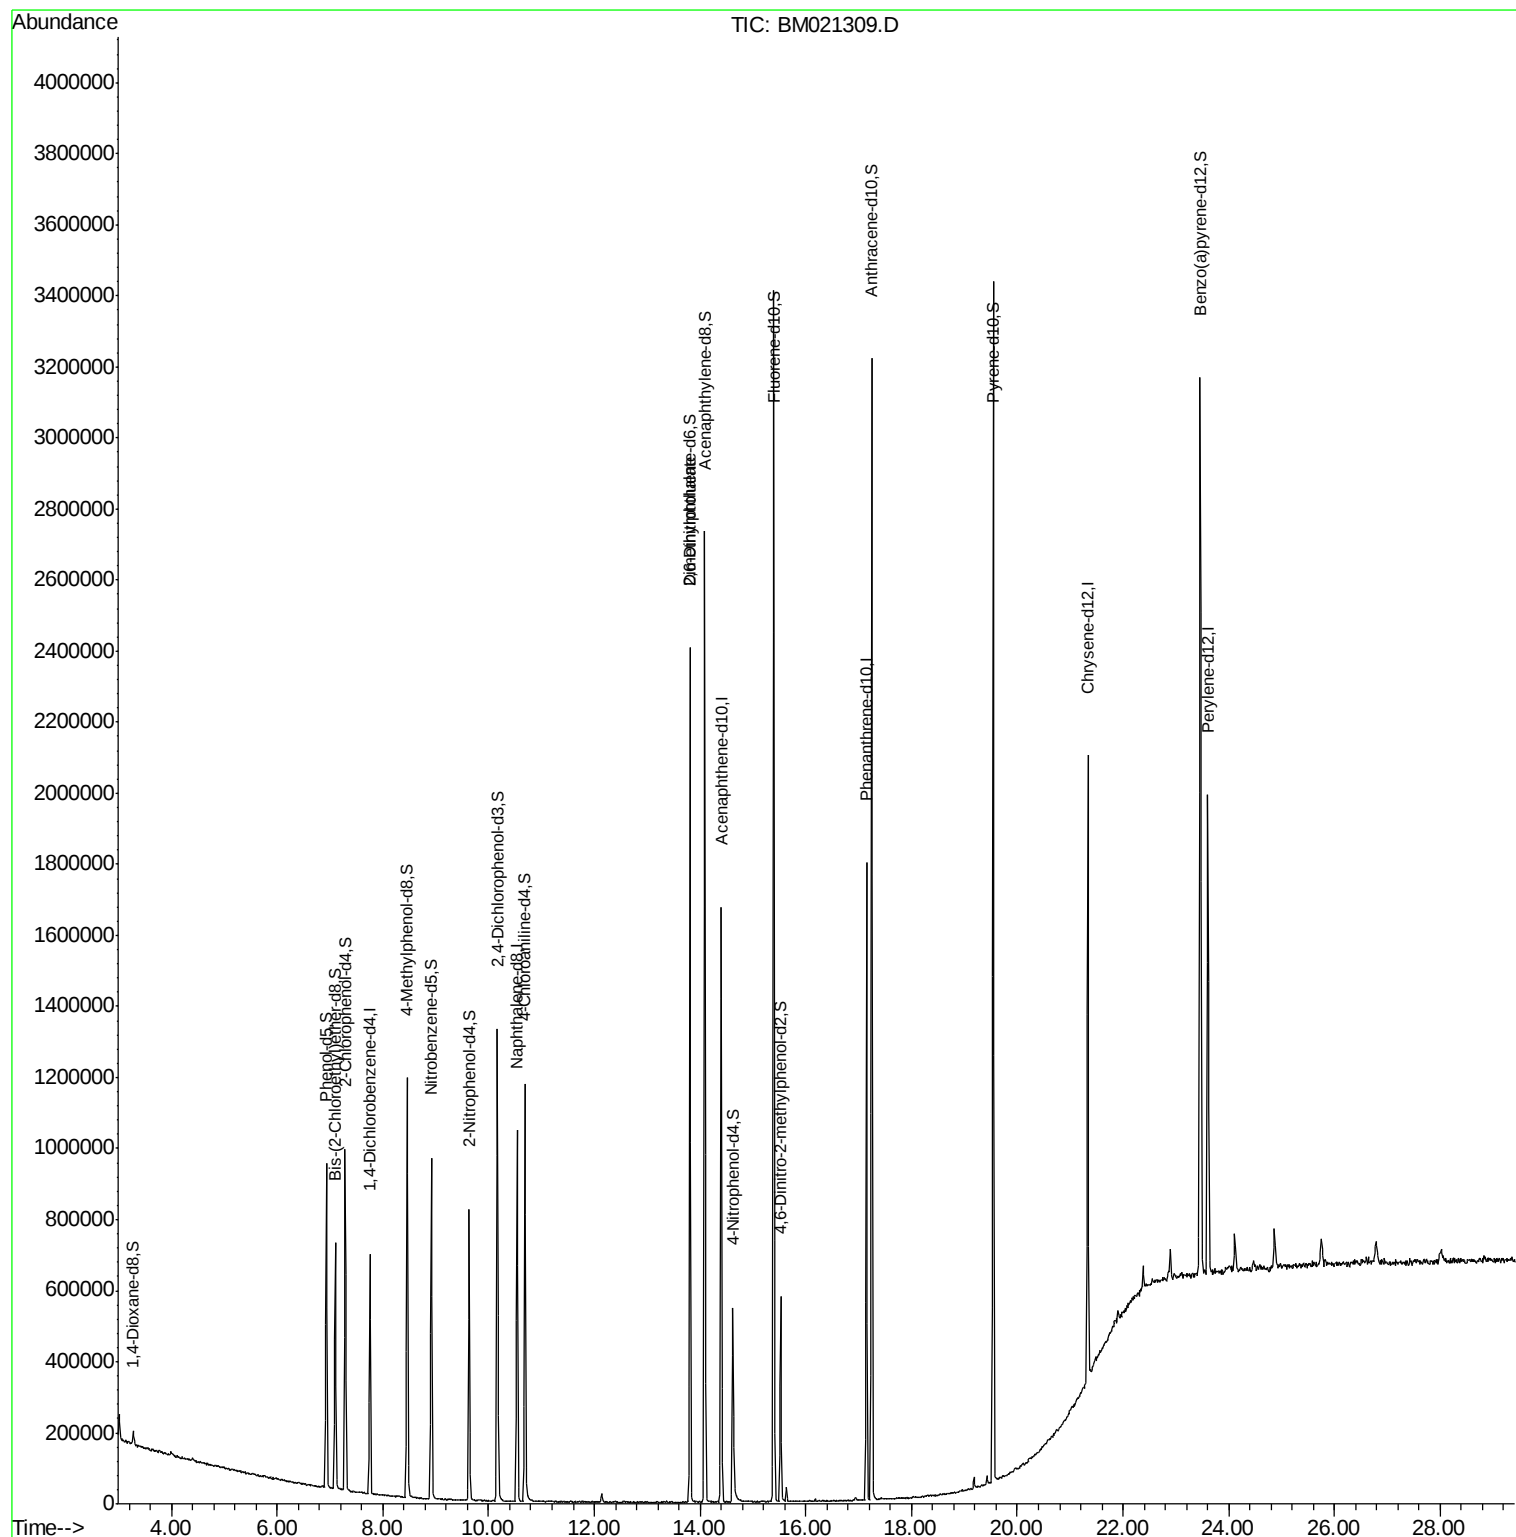

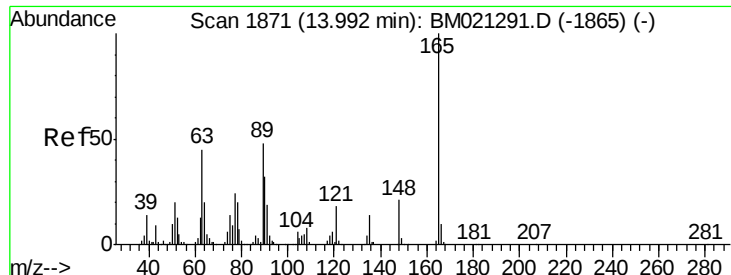

#45

2,6-Dinitrotoluene

Concen: 1.373 ng/ul

RT: 13.82 min Scan# 1841

Delta R.T. -0.18 min

Lab File: BM021309.D

Acq: 01 Jul 2019 15:02

Instrument :

BNA_M

ClientSampleId :

SBLK37



Tgt Ion:165 Resp: 11584

Ion Ratio Lower Upper

165 100

89 0.0 43.6 65.4#

121 24.3 16.5 24.7

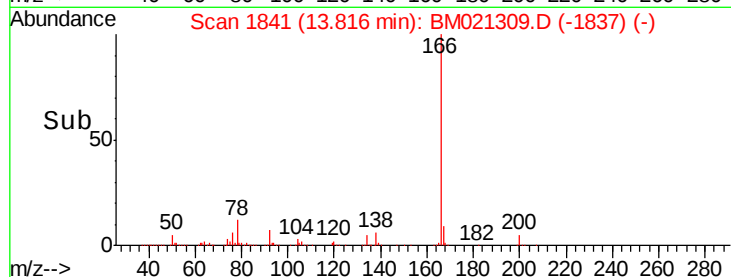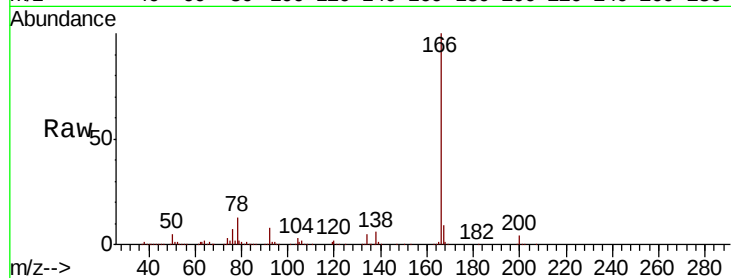

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

