

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070119\
 Data File : BM021314.D
 Acq On : 01 Jul 2019 18:04
 Operator : HP/JU
 Sample : K3578-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJG7

Quant Time: Jul 02 00:55:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 01 01:16:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	231426	20.00	ng/ul	0.00
18) Naphthalene-d8	10.54	136	1037097	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	662286	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1389049	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	993311	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1172731	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	26471	5.43	ng/uL	0.00
5) Phenol-d5	6.93	99	139274	6.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	349495	29.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	422148	25.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	285463	16.98	ng/ul	-0.01
19) Nitrobenzene-d5	8.92	128	281595	33.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	331777	35.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	608949	32.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	58101	2.93	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	2087301	34.88	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	2457158	33.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	43946	4.51	ng/ul	0.00
57) Fluorene-d10	15.39	176	1774395	34.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	246466	28.86	ng/ul	0.00
70) Anthracene-d10	17.24	188	2561324	35.48	ng/ul	0.00
78) Pyrene-d10	19.54	212	2341126	39.28	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	2494718	36.06	ng/ul	0.00


Target Compounds					Qvalue
17) Hexachloroethane	8.85	117	30694	4.774 ng/ul#	1
44) Dimethylphthalate	13.86	163	86305	1.584 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070119\
Data File : BM021314.D
Acq On : 01 Jul 2019 18:04
Operator : HP/JU
Sample : K3578-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJG7

Quant Time: Jul 02 00:55:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 01 01:16:07 2019
Response via : Initial Calibration

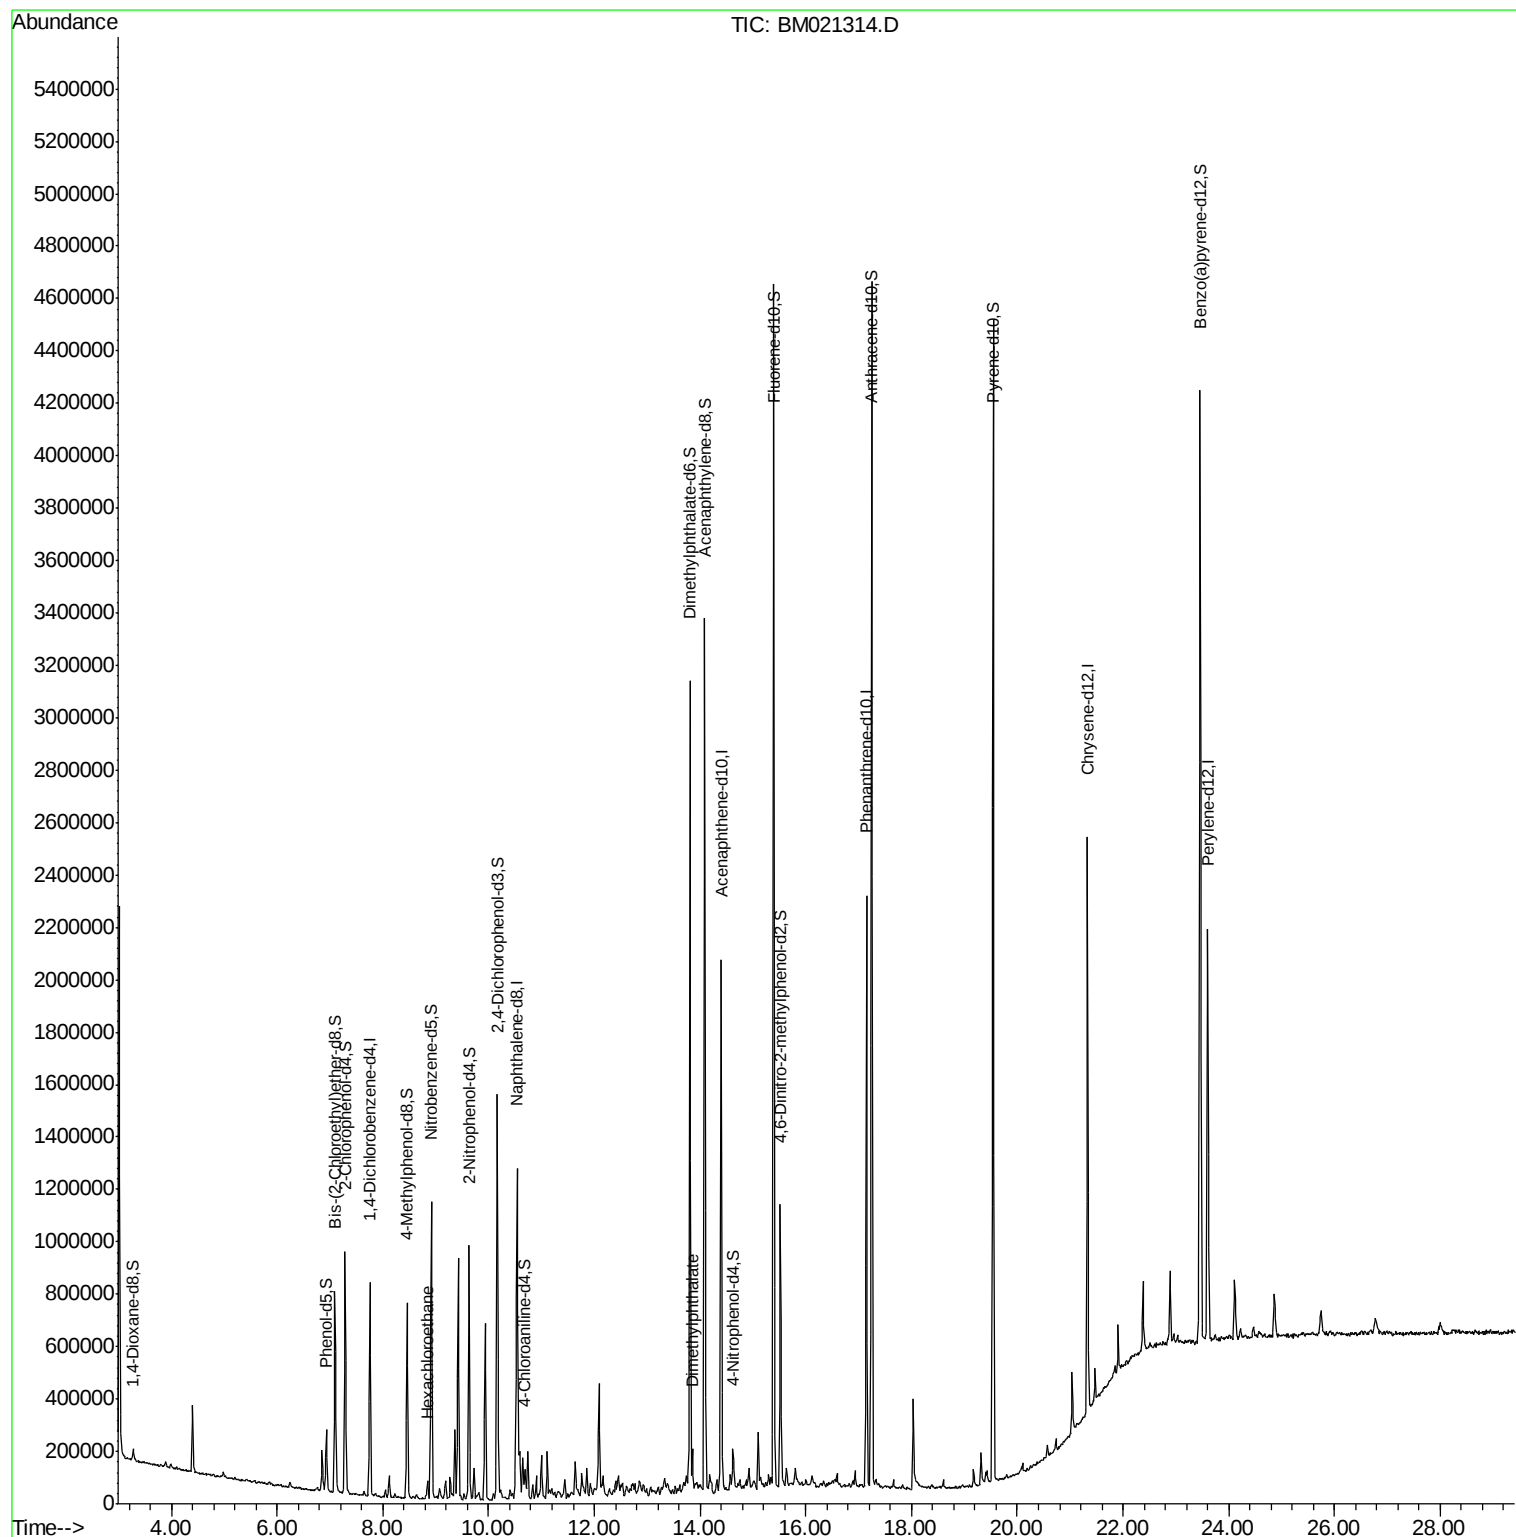


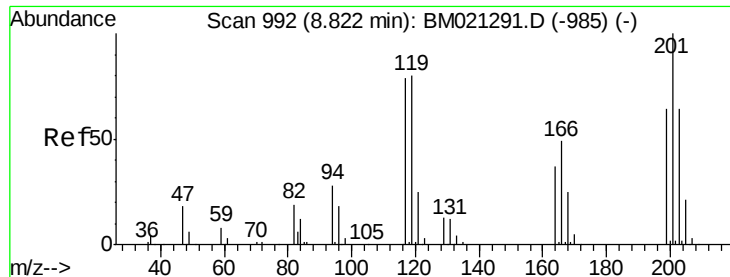




#17
Hexachloroethane
Concen: 4.774 ng/ul
RT: 8.85 min Scan# 997
Delta R.T. 0.03 min
Lab File: BM021314.D
Acq: 01 Jul 2019 18:04

Instrument :
BNA_M
ClientSampled :
JLJG7

Tgt Ion:117 Resp: 30694
Ion Ratio Lower Upper
117 100
201 0.0 93.9 140.9#
199 0.0 57.8 86.8#

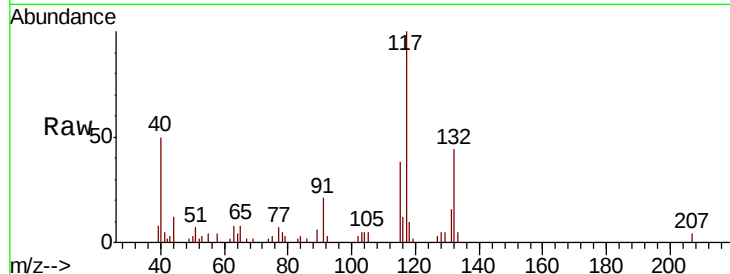


Abundance Ion 117.00 (116.70 to 117.70): E
Ion 201.00 (200.70 to 201.70): E
Ion 199.00 (198.70 to 199.70): E

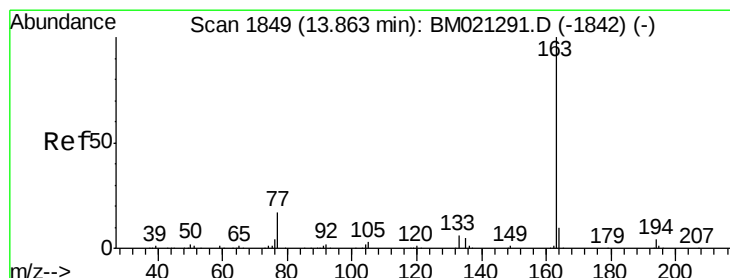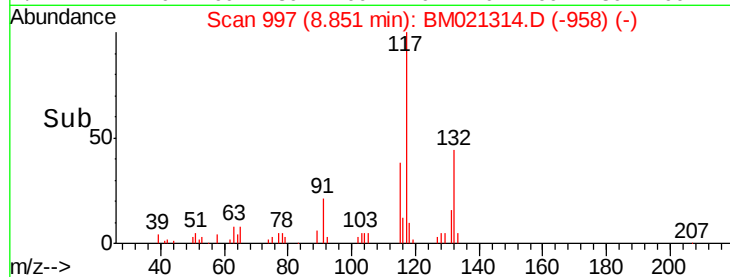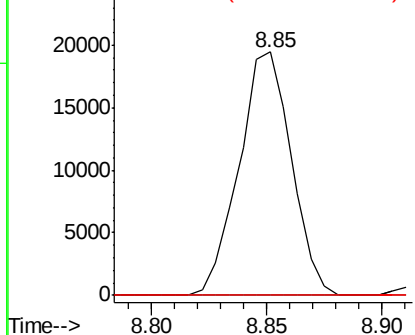

#44
Dimethylphthalate
Concen: 1.584 ng/ul
RT: 13.86 min Scan# 1848
Delta R.T. -0.01 min
Lab File: BM021314.D
Acq: 01 Jul 2019 18:04

Tgt Ion:163 Resp: 86305
Ion Ratio Lower Upper
163 100
194 4.5 3.4 5.2
164 10.2 7.7 11.5

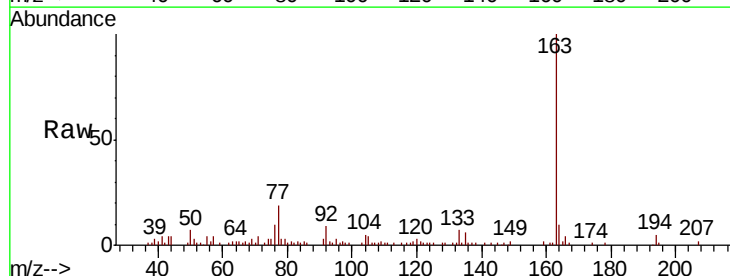

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

