

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070119\
 Data File : BM021317.D
 Acq On : 01 Jul 2019 19:53
 Operator : HP/JU
 Sample : K3578-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJG6

Quant Time: Jul 02 00:56:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 01 01:16:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	255944	20.00	ng/ul	0.00
18) Naphthalene-d8	10.54	136	1127268	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	717330	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1509182	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	1077361	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1281503	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	28464	5.28	ng/uL	0.00
5) Phenol-d5	6.93	99	152472	6.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	384303	28.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	463747	25.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	309303	16.63	ng/ul	-0.01
19) Nitrobenzene-d5	8.92	128	303869	33.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	360493	35.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	657150	31.81	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	24163	1.12	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	2203459	34.00	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	2598408	32.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	49112	4.66	ng/ul	0.00
57) Fluorene-d10	15.39	176	1875698	33.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	273100	29.44	ng/ul	0.00
70) Anthracene-d10	17.24	188	2654989	33.85	ng/ul	0.00
78) Pyrene-d10	19.54	212	2433332	37.64	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	2563507	33.91	ng/ul	0.00


Target Compounds					Qvalue	
17) Hexachloroethane	8.85	117	24852	3.495	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070119\
Data File : BM021317.D
Acq On : 01 Jul 2019 19:53
Operator : HP/JU
Sample : K3578-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJG6

Quant Time: Jul 02 00:56:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 01 01:16:07 2019
Response via : Initial Calibration

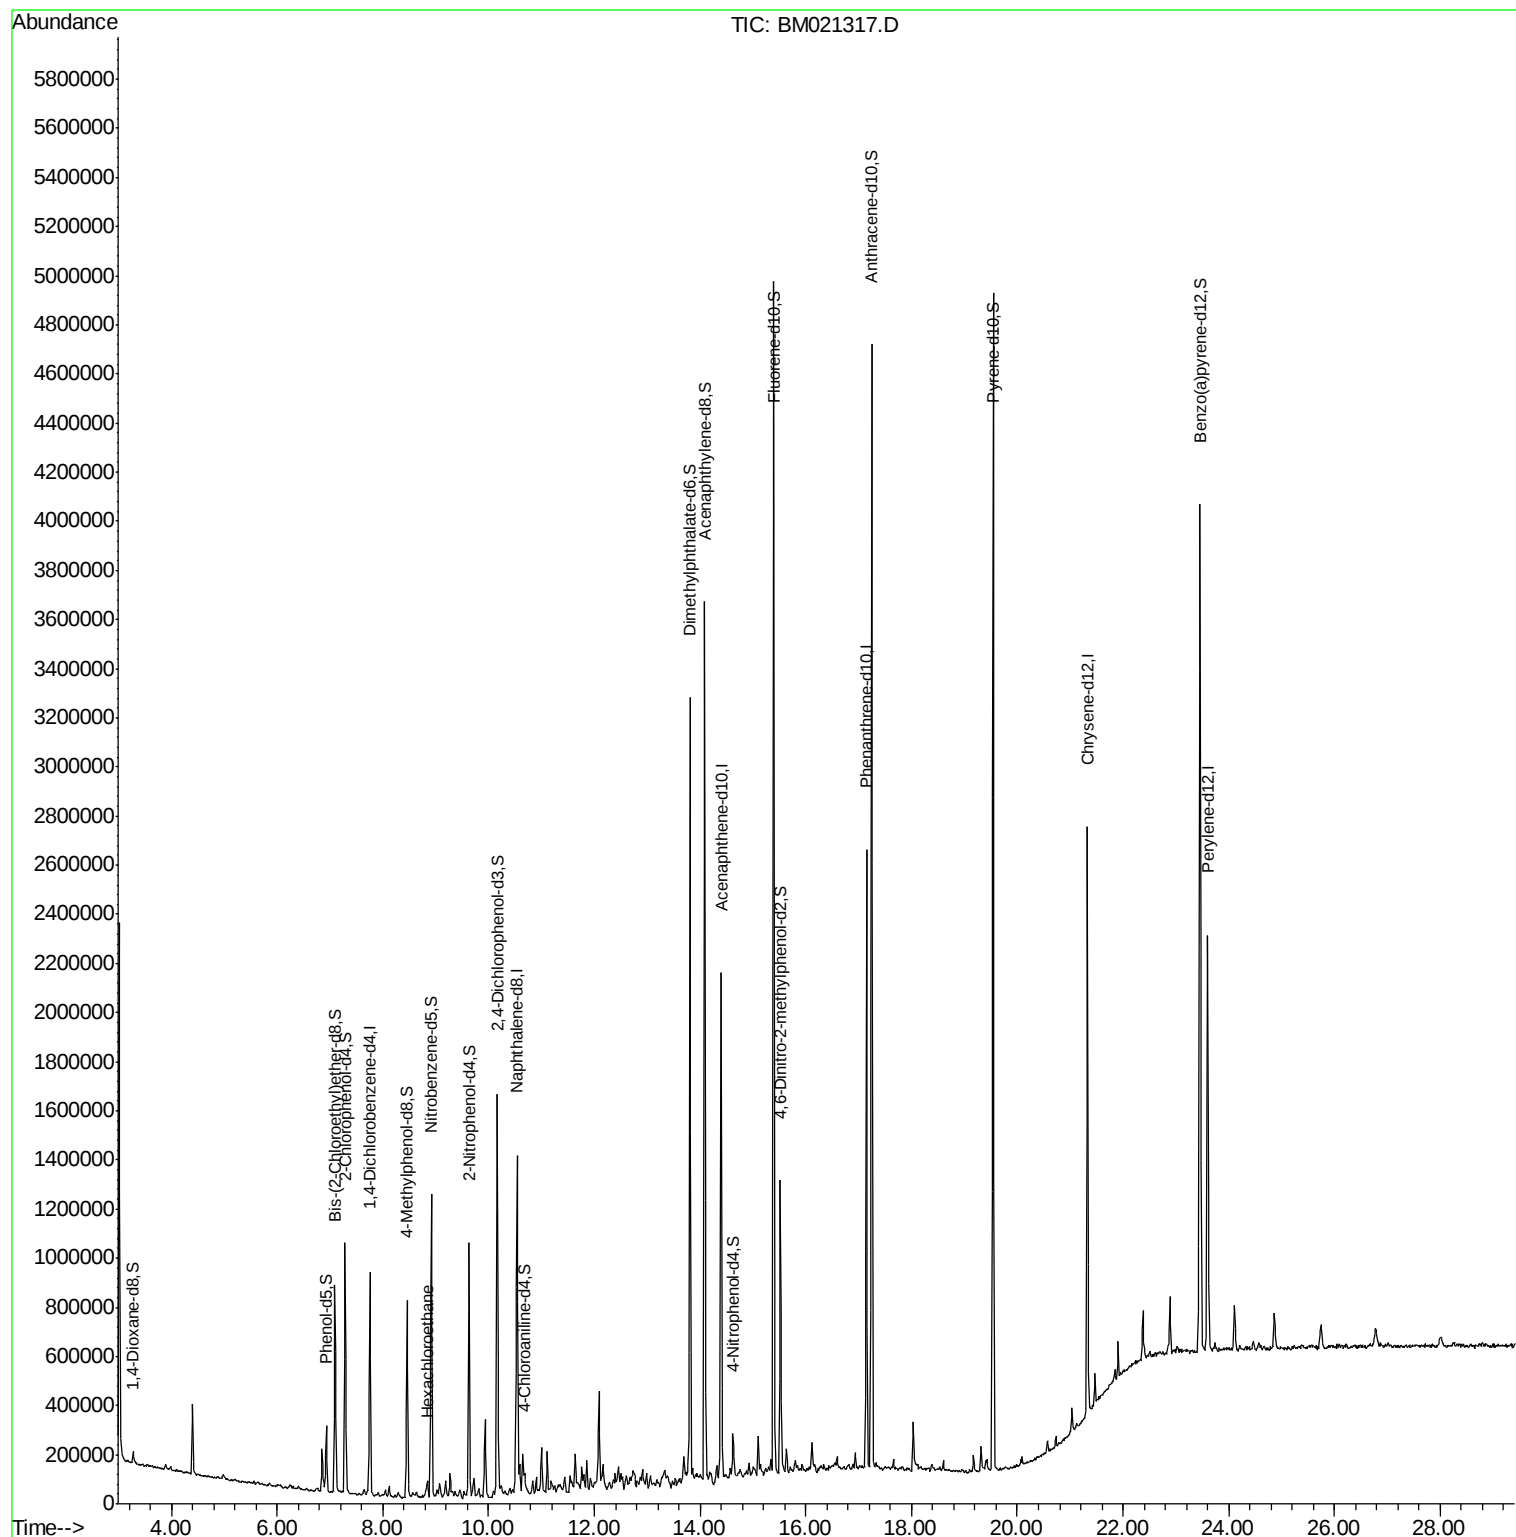

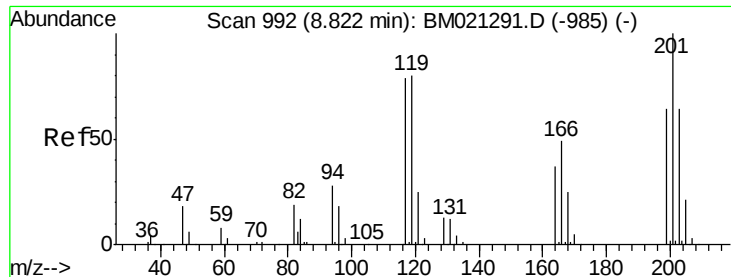

#17
 Hexachloroethane
 Concen: 3.495 ng/ul
 RT: 8.85 min Scan# 997
 Delta R.T. 0.03 min
 Lab File: BM021317.D
 Acq: 01 Jul 2019 19:53

Instrument :
 BNA_M
 ClientSampleId :
 JLJG6

Tgt Ion	Ratio	Lower	Upper
117	100		
201	0.0	93.9	140.9#
199	0.0	57.8	86.8#

