

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070119\
 Data File : BM021326.D
 Acq On : 02 Jul 2019 01:56
 Operator : HP/JU
 Sample : K3562-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5AE6

Quant Time: Jul 02 04:17:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 02 01:54:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	251718	20.00	ng/ul	0.00
18) Naphthalene-d8	10.54	136	1129437	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	722657	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1557089	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	1112499	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1297512	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	30606	5.77	ng/uL	0.00
5) Phenol-d5	6.93	99	164744	7.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	363186	27.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	450222	25.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	318664	17.42	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	291693	31.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	343756	33.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	627131	30.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	76784	3.56	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	2162352	33.12	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	2561652	32.05	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	49833	4.69	ng/ul	0.01
57) Fluorene-d10	15.39	176	1889550	33.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	243801	25.47	ng/ul	0.00
70) Anthracene-d10	17.24	188	2809974	34.73	ng/ul	0.00
78) Pyrene-d10	19.54	212	2530001	37.90	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	2657573	34.72	ng/ul	0.00


Target Compounds					Qvalue	
45) 2,6-Dinitrotoluene	13.81	165	13952	1.230	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070119\
Data File : BM021326.D
Acq On : 02 Jul 2019 01:56
Operator : HP/JU
Sample : K3562-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5AE6

Quant Time: Jul 02 04:17:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 02 01:54:12 2019
Response via : Initial Calibration

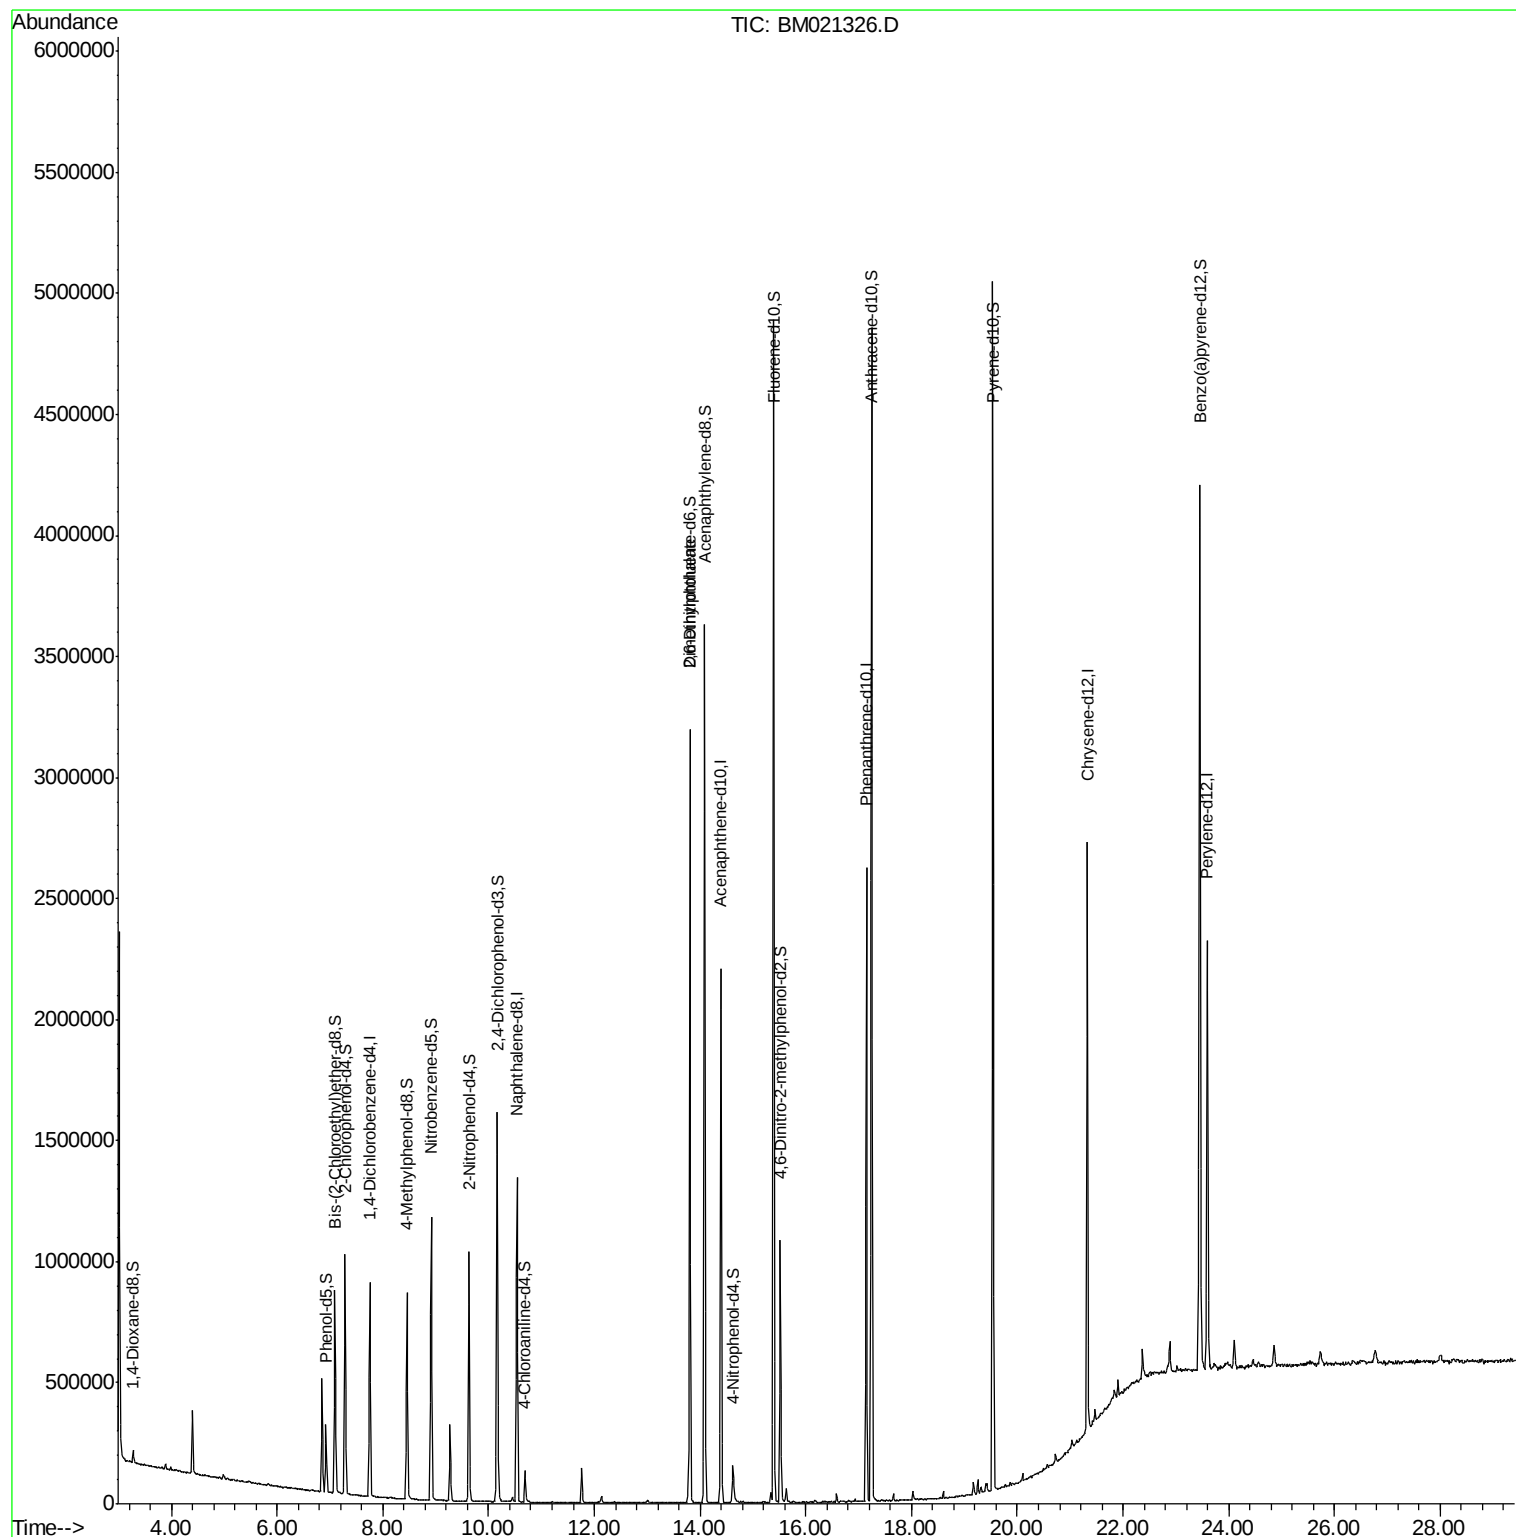

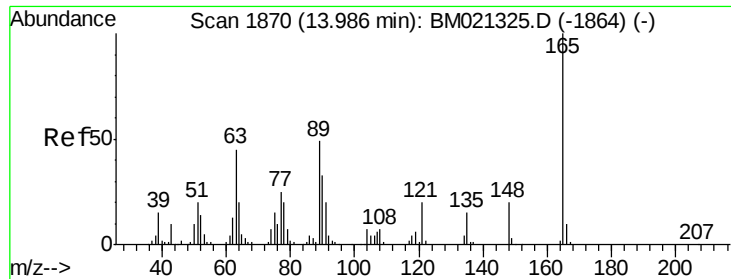

#45
 2,6-Dinitrotoluene
 Concen: 1.230 ng/ul
 RT: 13.81 min Scan# 1840
 Delta R.T. -0.18 min
 Lab File: BM021326.D
 Acq: 02 Jul 2019 01:56

Instrument :
 BNA_M
 ClientSampleId :
 C5AE6

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	43.6	65.4#
121	28.1	16.5	24.7#

