

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070119\
 Data File : BM021322.D
 Acq On : 01 Jul 2019 22:54
 Operator : HP/JU
 Sample : K3578-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJG8

Quant Time: Jul 02 00:56:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 01 01:16:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	225843	20.00	ng/ul	0.00
18) Naphthalene-d8	10.54	136	1015466	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	655173	20.00	ng/ul	-0.01
61) Phenanthrene-d10	17.14	188	1418997	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	1005649	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1178594	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	26998	5.68	ng/uL	0.00
5) Phenol-d5	6.93	99	143568	7.30	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	301209	25.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	377756	23.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	272771	16.62	ng/ul	-0.01
19) Nitrobenzene-d5	8.92	128	242225	29.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	282722	30.89	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	535138	28.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	70686	3.64	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	1802947	30.46	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	2135468	29.47	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	40431	4.20	ng/ul	0.00
57) Fluorene-d10	15.39	176	1566569	30.42	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	204309	23.42	ng/ul	0.00
70) Anthracene-d10	17.24	188	2324750	31.53	ng/ul	0.00
78) Pyrene-d10	19.54	212	2116587	35.07	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	2195092	31.57	ng/ul	-0.01


Target Compounds					Ovalue	
44) Dimethylphthalate	13.86	163	80088	1.486	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070119\
Data File : BM021322.D
Acq On : 01 Jul 2019 22:54
Operator : HP/JU
Sample : K3578-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJG8

Quant Time: Jul 02 00:56:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 01 01:16:07 2019
Response via : Initial Calibration

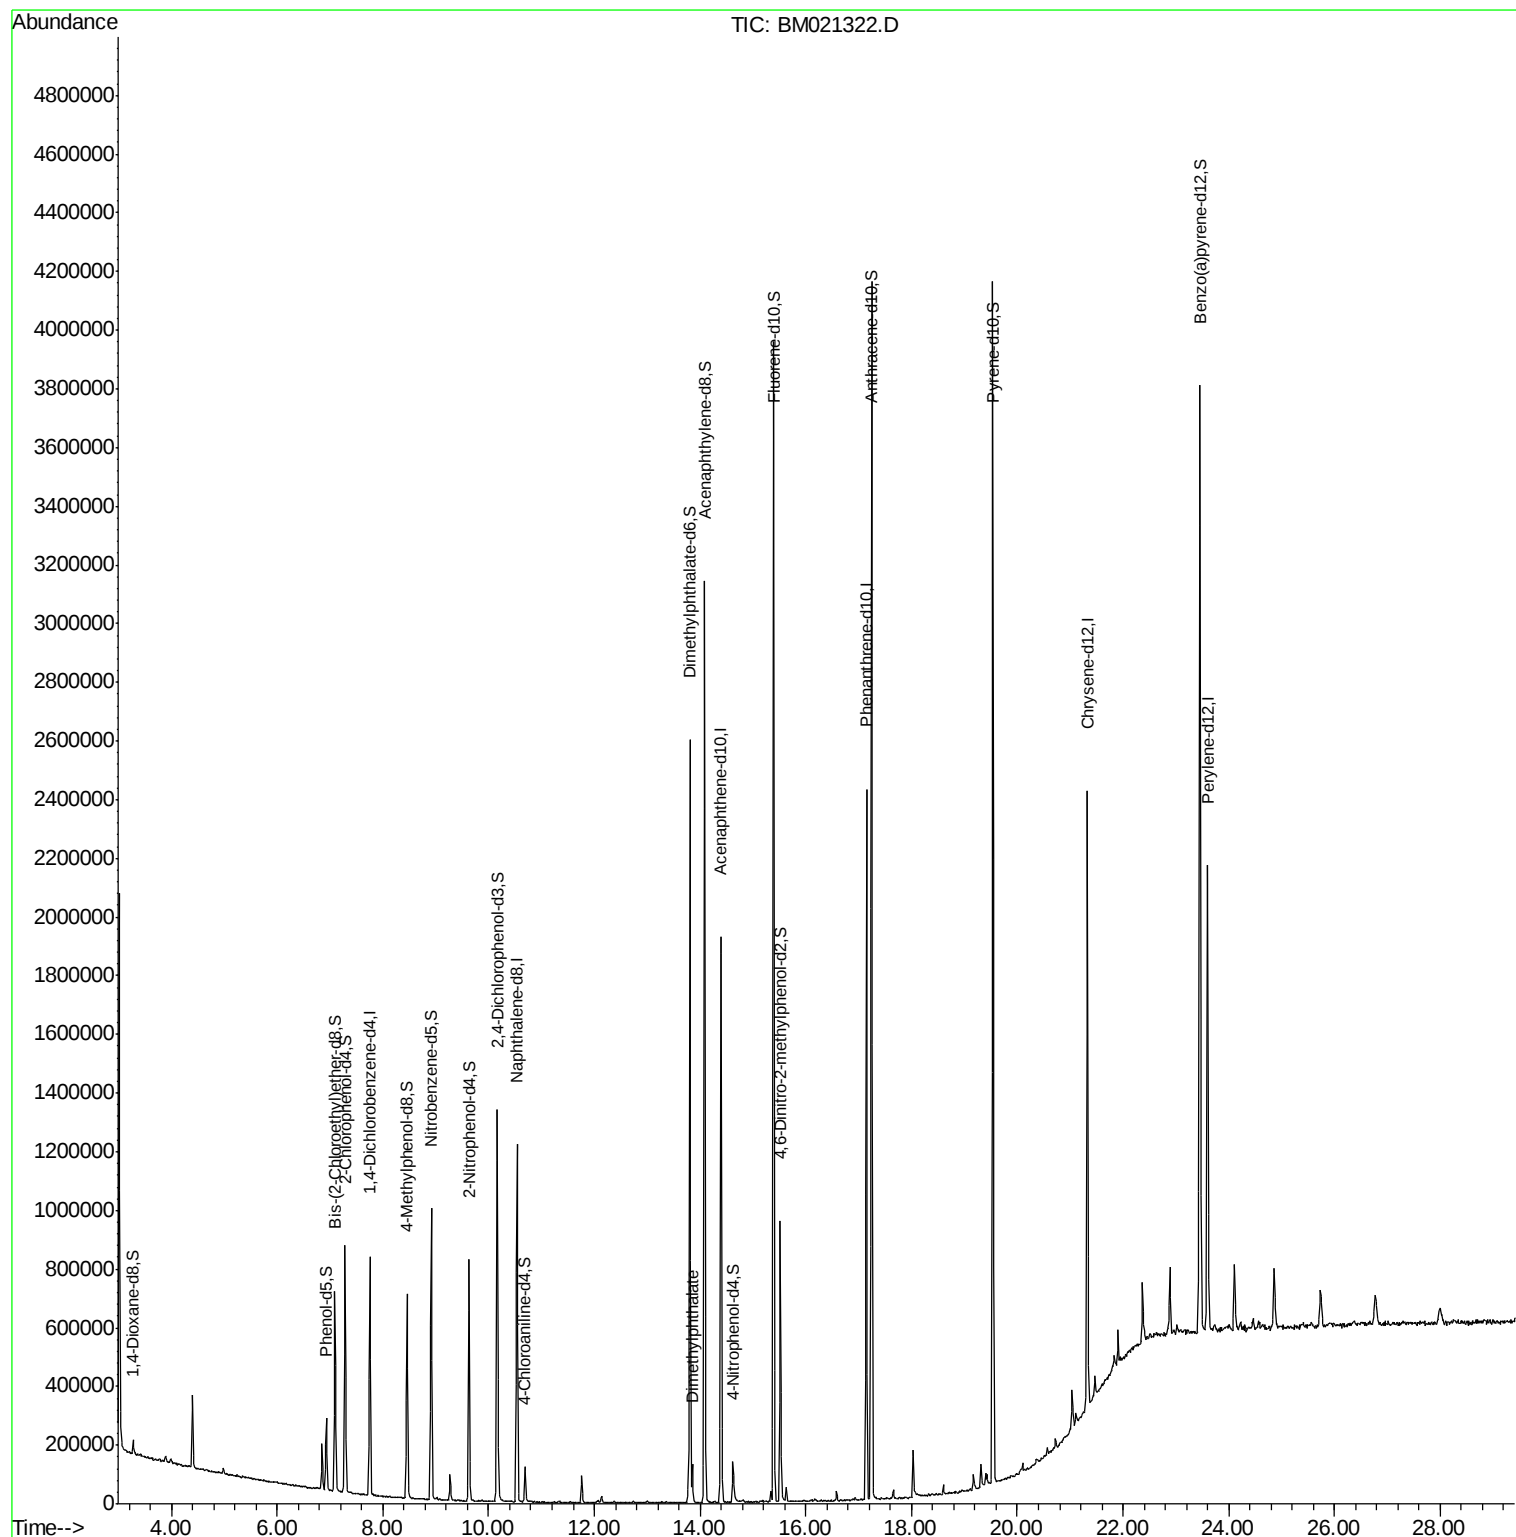

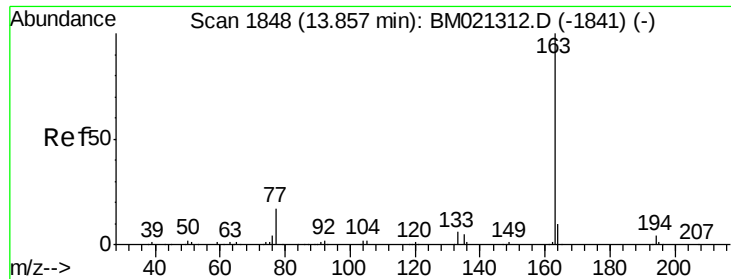

#44

Dimethylphthalate

Concen: 1.486 ng/ul

RT: 13.86 min Scan# 1848

Delta R.T. -0.01 min

Lab File: BM021322.D

Acq: 01 Jul 2019 22:54

Instrument :

BNA_M

ClientSampleId :

JLJG8


Tot Ion:163 Resp: 80088

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2

164 10.4 7.7 11.5

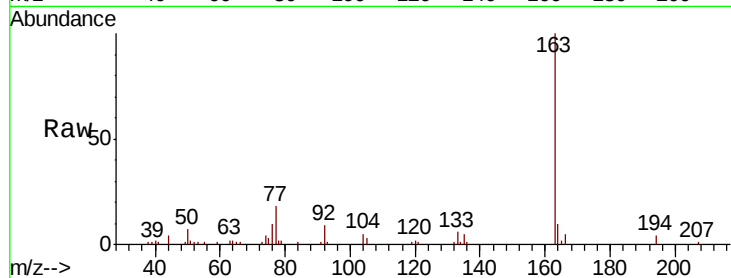

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

