

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070119\
 Data File : BM021328.D
 Acq On : 02 Jul 2019 03:08
 Operator : HP/JU
 Sample : K3562-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5AE7

Quant Time: Jul 02 04:17:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 02 01:54:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	242555	20.00	ng/ul	0.00
18) Naphthalene-d8	10.54	136	1077019	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	680012	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1411581	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	1083563	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1288539	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	29458	5.77	ng/uL	0.00
5) Phenol-d5	6.92	99	149690	7.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	353456	28.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	428753	24.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	292738	16.61	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	279038	31.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	327673	33.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	611526	30.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	74692	3.63	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	2148748	34.97	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	2503075	33.28	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	40912	4.09	ng/ul	0.01
57) Fluorene-d10	15.39	176	1824674	34.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	224709	25.90	ng/ul	0.00
70) Anthracene-d10	17.24	188	2620180	35.72	ng/ul	0.00
78) Pyrene-d10	19.54	212	2458935	37.82	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	2720236	35.78	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.85	163	85101	1.521	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070119\
Data File : BM021328.D
Acq On : 02 Jul 2019 03:08
Operator : HP/JU
Sample : K3562-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5AE7

Quant Time: Jul 02 04:17:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 02 01:54:12 2019
Response via : Initial Calibration

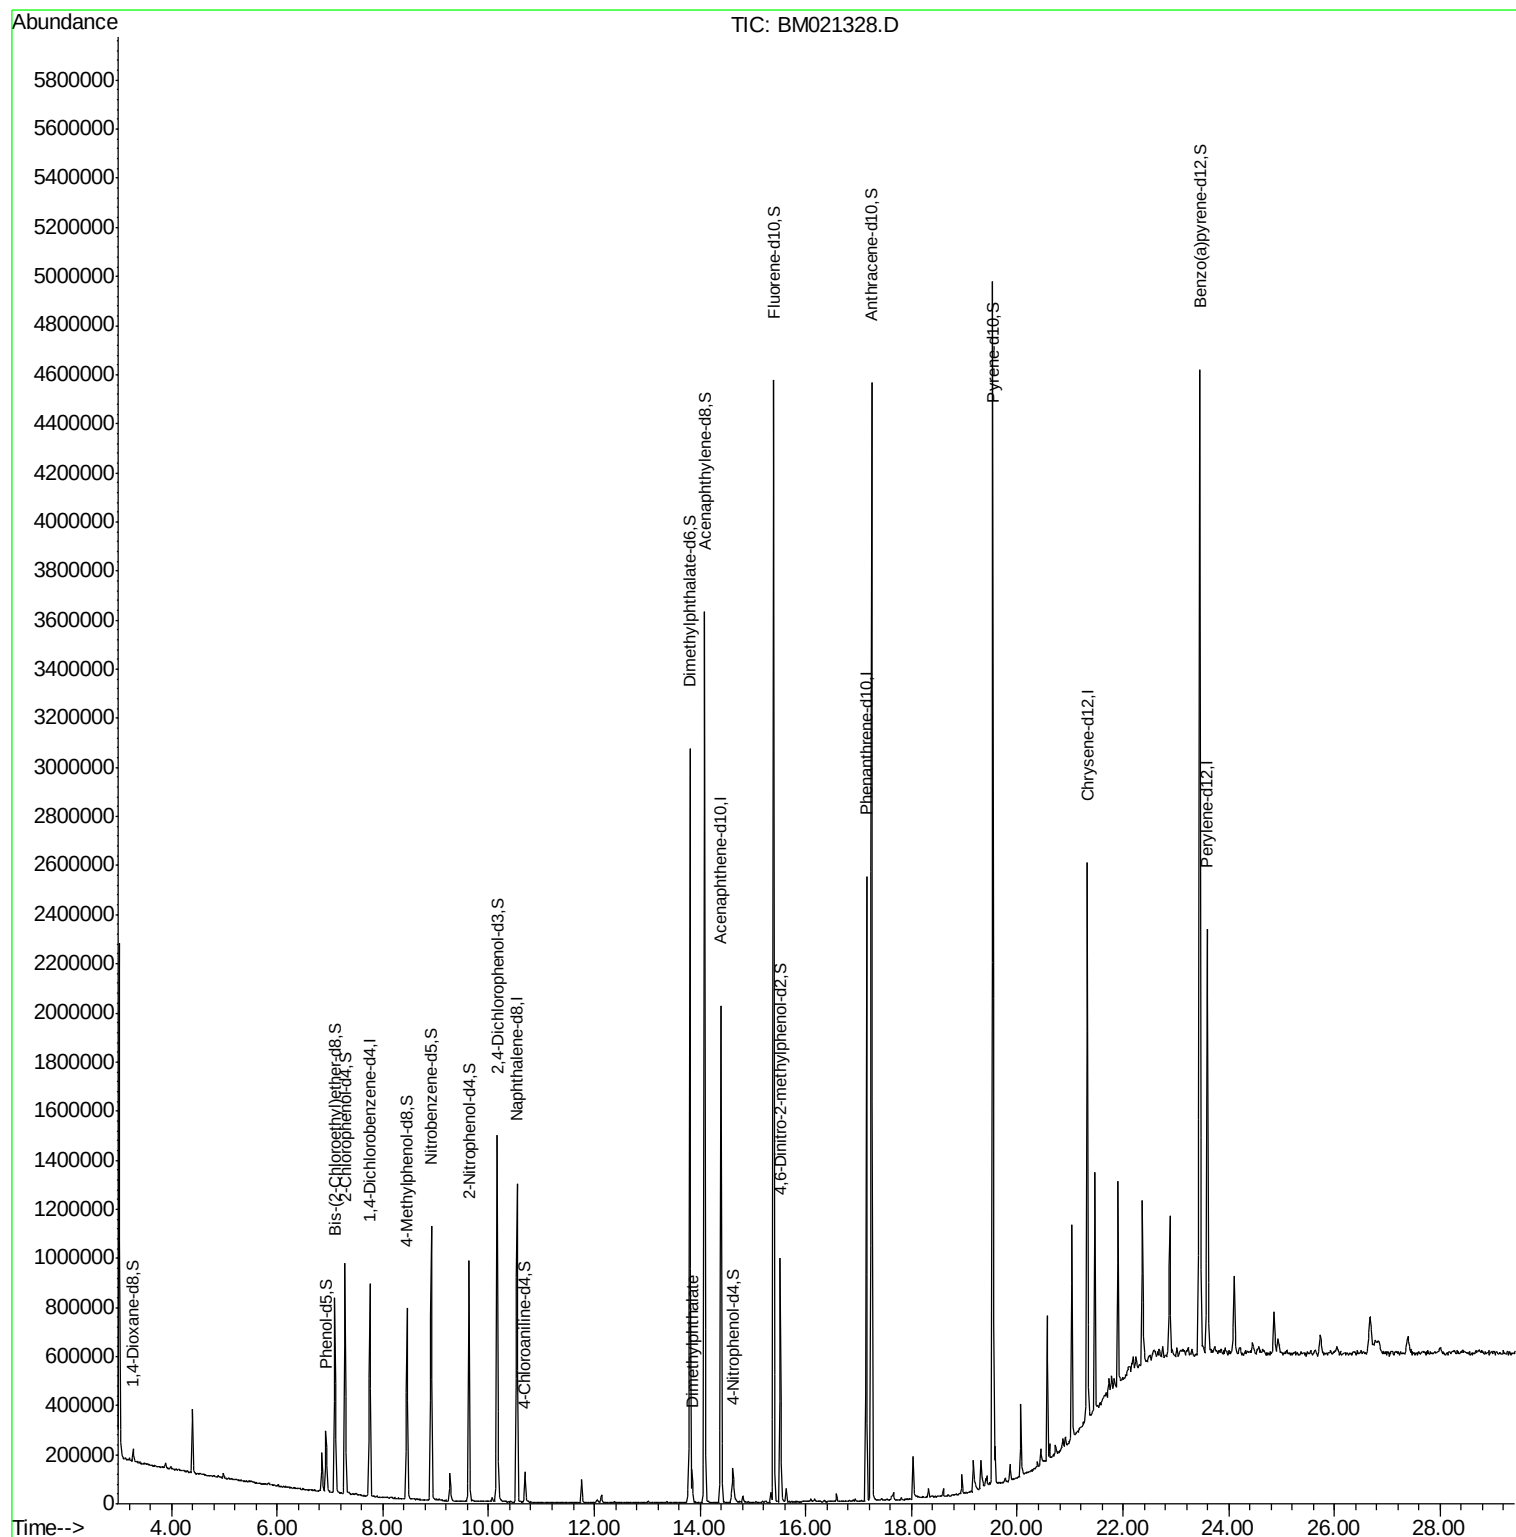

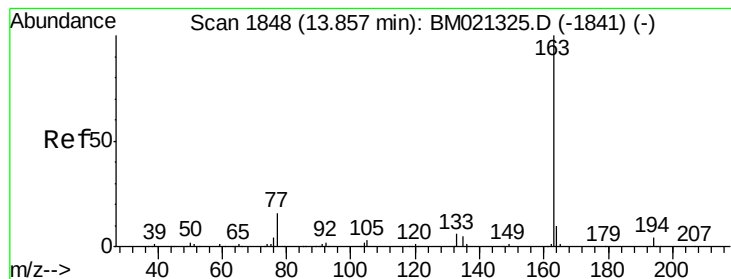

#44

Dimethylphthalate

Concen: 1.521 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BM021328.D

Acq: 02 Jul 2019 03:08

Instrument :

BNA_M

ClientSampleId :

C5AE7


Tot Ion:163 Resp: 85101

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2

164 11.2 7.7 11.5

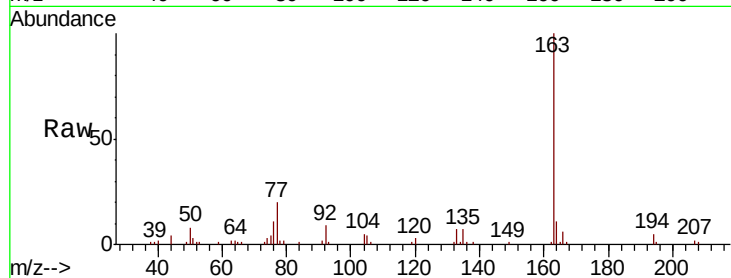

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

