

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070123\
 Data File : BM040520.D
 Acq On : 02 Jul 2023 02:04
 Operator : MA/JU
 Sample : 03242-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCGB0

Quant Time: Jul 02 05:17:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 03:00:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.932	152	8346	0.400	ng/ul	0.00
4) Naphthalene-d8	10.740	136	30650	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.572	164	17368	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.320	188	36342	0.400	ng/ul	0.00
17) Chrysene-d12	21.503	240	25099	0.400	ng/ul	0.00
23) Perylene-d12	23.915	264	23222	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	47509	3.624	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.329	152	11110	0.259	ng/ul	0.00
18) Fluoranthene-d10	19.352	212	22411	0.279	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.789	128	2465	0.029	ng/ul#	75
7) 2-Methylnaphthalene	12.400	142	1583	0.032	ng/ul	94
8) 1-Methylnaphthalene	12.620	142	1159	0.023	ng/ul	96
10) Acenaphthylene	14.295	152	2202	0.028	ng/ul#	76
15) Phenanthrene	17.362	178	19837	0.176	ng/ul	99
16) Anthracene	17.455	178	2922	0.031	ng/ul#	80
19) Fluoranthene	19.380	202	53439	0.501	ng/ul	99
20) Pyrene	19.742	202	43903	0.384	ng/ul	97
21) Benzo(a)anthracene	21.486	228	22892	0.270	ng/ul	94
22) Chrysene	21.541	228	29964	0.309	ng/ul#	96
24) Benzo(b)fluoranthene	23.181	252	42505	0.473	ng/ul	91
26) Benzo(a)pyrene	23.803	252	24520	0.303	ng/ul#	88
27) Indeno(1,2,3-cd)pyrene	26.417	276	23643	0.210	ng/ul#	79
28) Dibenzo(a,h)anthracene	26.427	278	5577	0.063	ng/ul#	43
29) Benzo(g,h,i)perylene	27.195	276	22406	0.227	ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070123\
Data File : BM040520.D
Acq On : 02 Jul 2023 02:04
Operator : MA/JU
Sample : 03242-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCGB0

Quant Time: Jul 02 05:17:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 03:00:05 2023
Response via : Initial Calibration




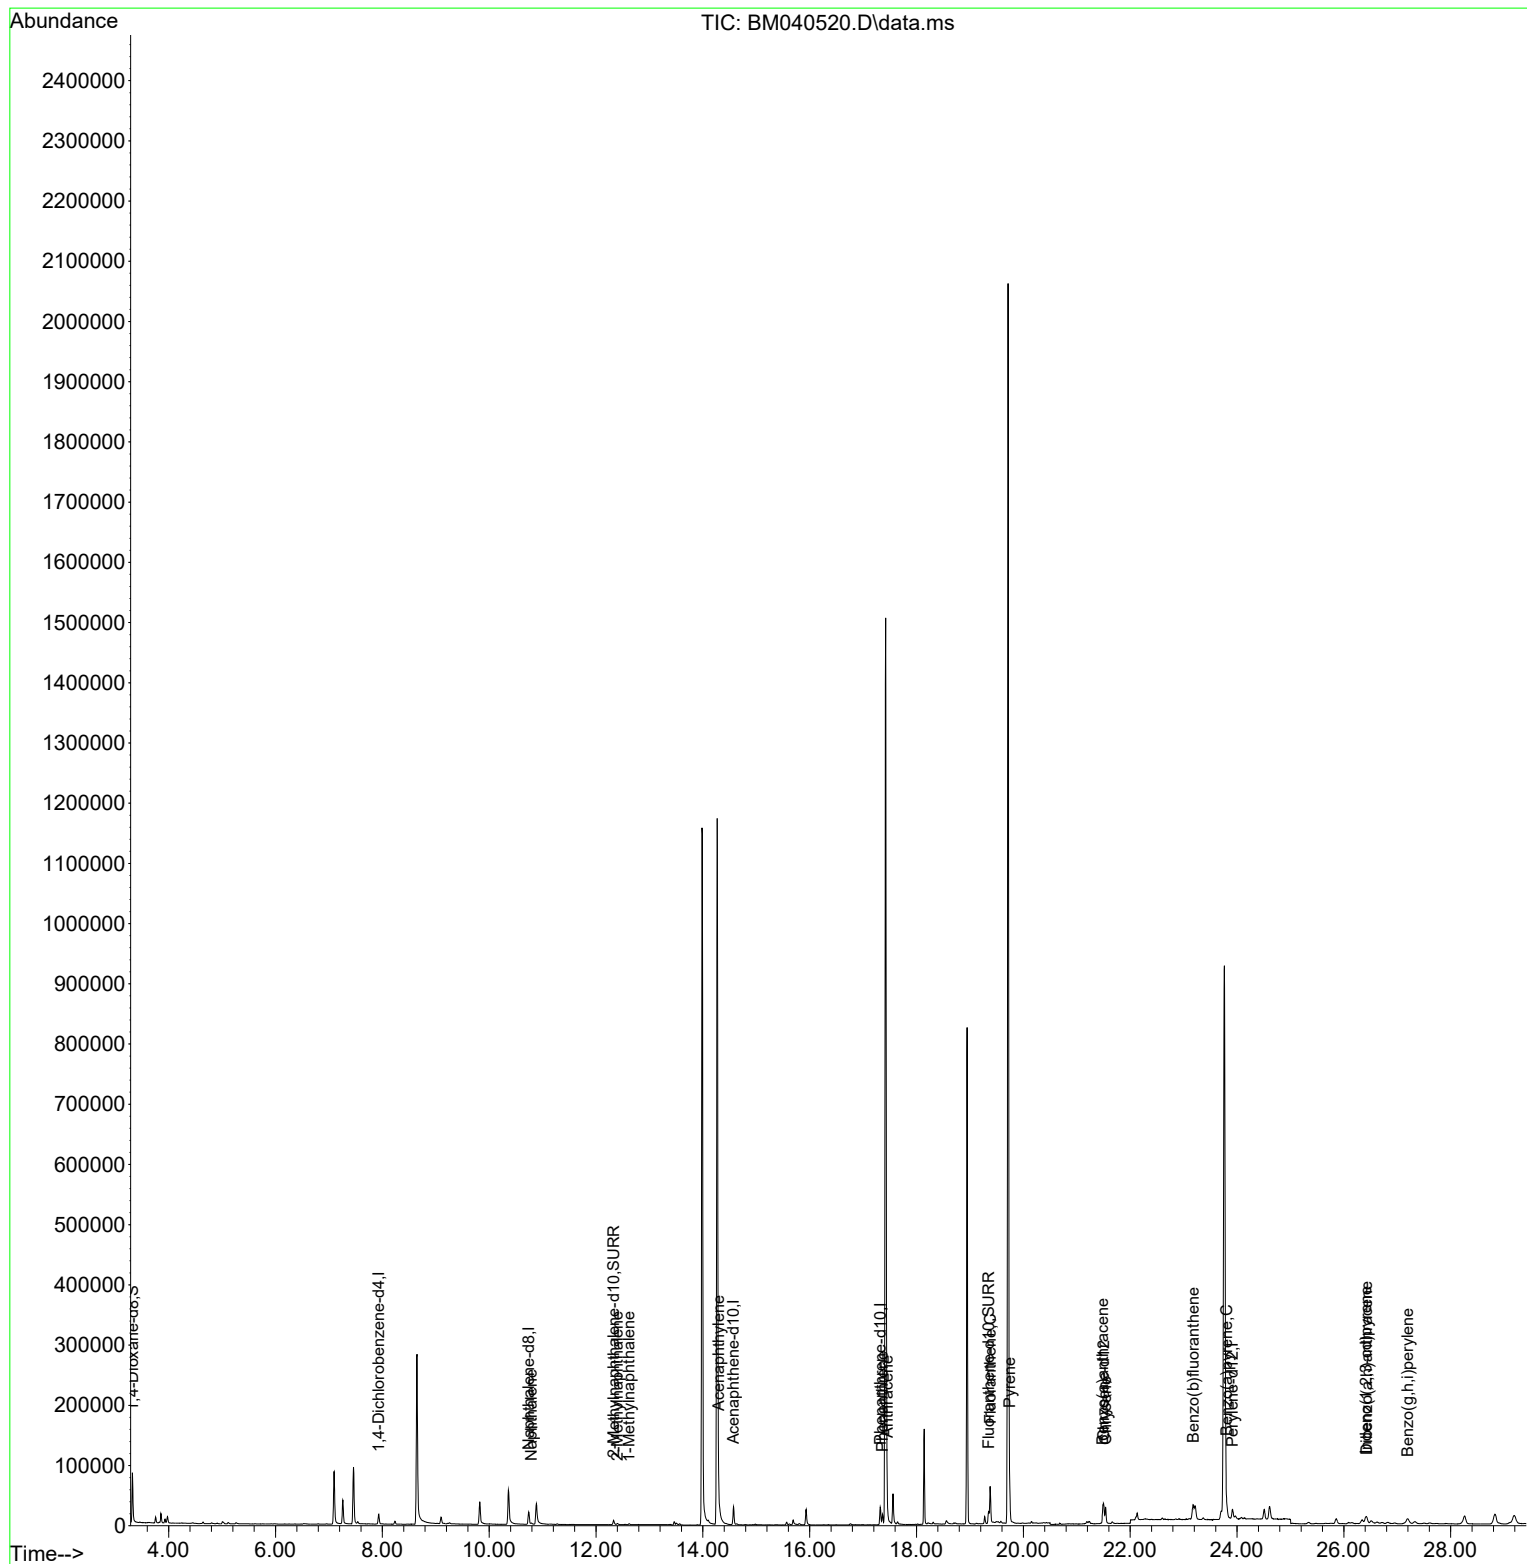


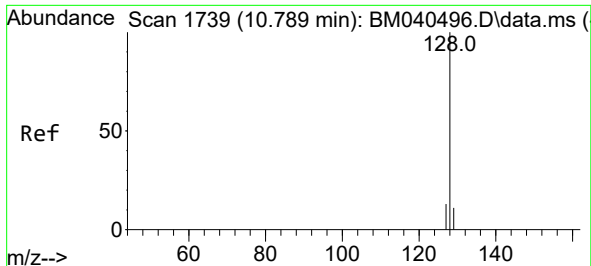

#5
Naphthalene
Concen: 0.029 ng/ul
RT: 10.789 min Scan# 1739
Delta R.T. -0.005 min
Lab File: BM040520.D
Acq: 02 Jul 2023 02:04




Instrument :
BNA_M
ClientSampleId :
DCGB0


Tgt Ion:128 Resp: 2465
Ion Ratio Lower Upper
128 100
129 26.8 9.2 13.8#
127 18.2 10.6 15.8#

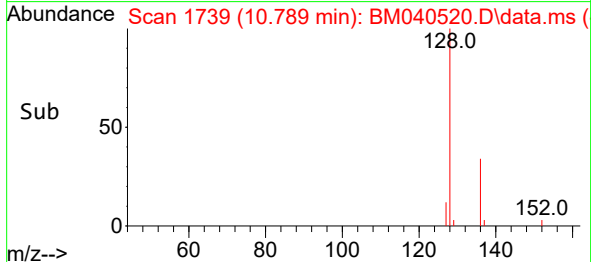

#7
2-Methylnaphthalene
Concen: 0.032 ng/ul
RT: 12.400 min Scan# 2032
Delta R.T. -0.005 min
Lab File: BM040520.D
Acq: 02 Jul 2023 02:04

Tgt Ion:142 Resp: 1583
Ion Ratio Lower Upper
142 100
141 95.1 71.9 107.9

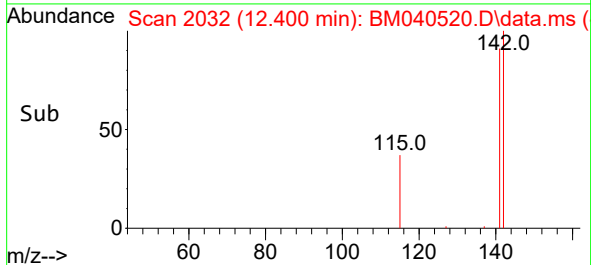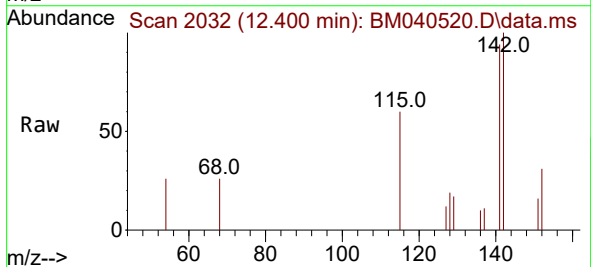



#8

1-Methylnaphthalene

Concen: 0.023 ng/ul

RT: 12.620 min Scan# 2072

Delta R.T. -0.005 min

Lab File: BM040520.D

Acq: 02 Jul 2023 02:04

Instrument :

BNA_M

ClientSampleId :





DCGB0

Tgt Ion:142 Resp: 1159

Ion Ratio Lower Upper

142 100

141 95.9 73.7 110.5

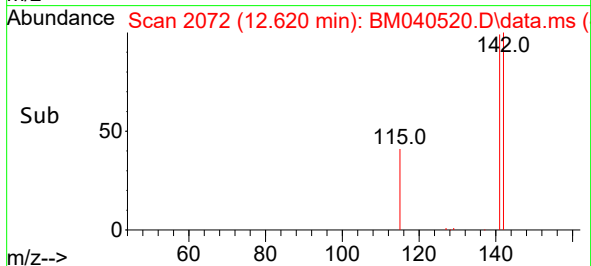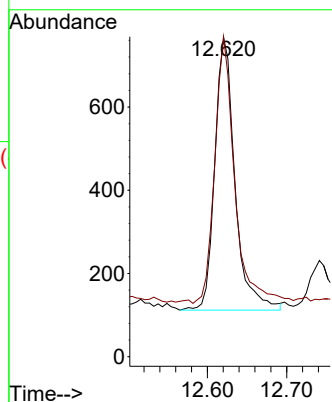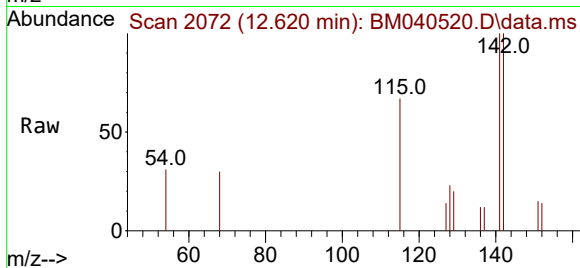

#10

Acenaphthylene

Concen: 0.028 ng/ul

RT: 14.295 min Scan# 2407

Delta R.T. -0.004 min

Lab File: BM040520.D

Acq: 02 Jul 2023 02:04




Tgt Ion:152 Resp: 2202


Ion Ratio Lower Upper

152 100

151 28.6 16.2 24.2#

153 27.2 10.9 16.3#


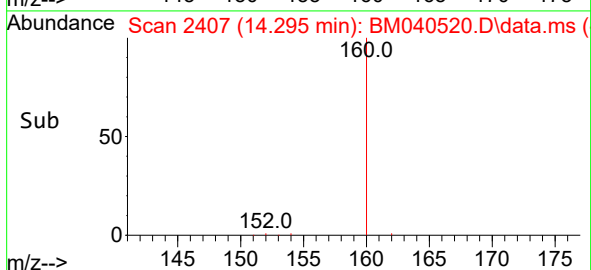

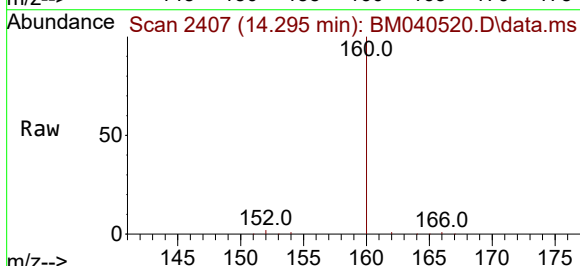


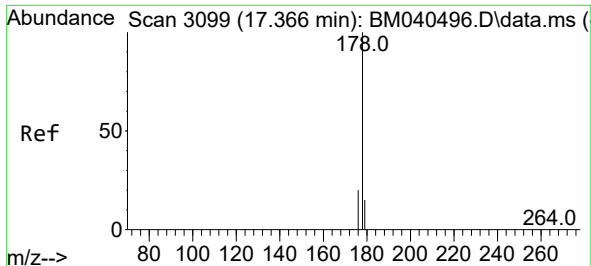

#15
Phenanthrene
Concen: 0.176 ng/ul
RT: 17.362 min Scan# 3099
Delta R.T. -0.008 min
Lab File: BM040520.D
Acq: 02 Jul 2023 02:04




Instrument :
BNA_M
ClientSampleId :
DCGB0


Tgt Ion:178 Resp: 19837
Ion Ratio Lower Upper
178 100
179 16.9 12.8 19.2
176 20.4 16.4 24.6

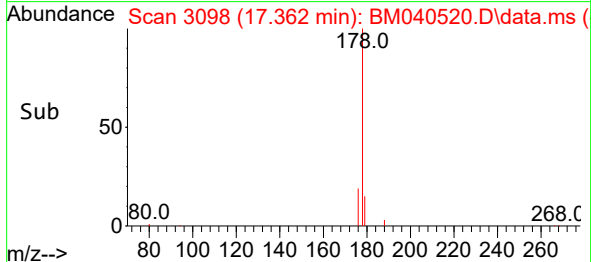

#16
Anthracene
Concen: 0.031 ng/ul
RT: 17.455 min Scan# 3120
Delta R.T. -0.008 min
Lab File: BM040520.D
Acq: 02 Jul 2023 02:04

Tgt Ion:178 Resp: 2922
Ion Ratio Lower Upper
178 100
179 27.1 12.9 19.3#
176 26.5 15.8 23.6#


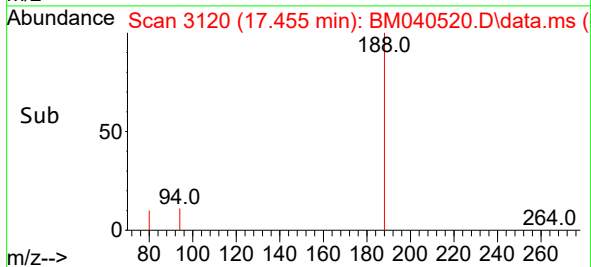

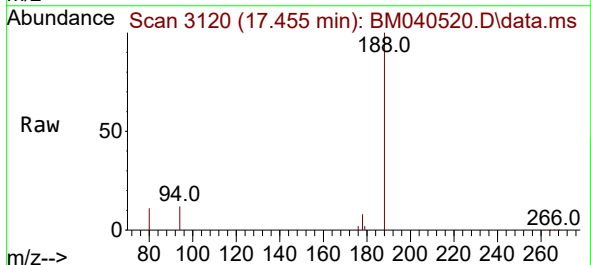


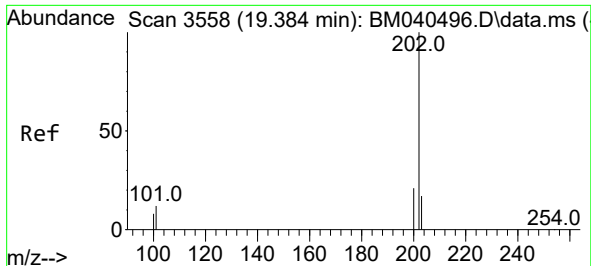

#19
Fluoranthene
Concen: 0.501 ng/ul
RT: 19.380 min Scan# 3558
Delta R.T. -0.005 min
Lab File: BM040520.D
Acq: 02 Jul 2023 02:04




Instrument :
BNA_M
ClientSampleId :
DCGB0


Tgt Ion:202 Resp: 53439
Ion Ratio Lower Upper
202 100
101 14.0 11.4 17.0
100 10.1 8.7 13.1

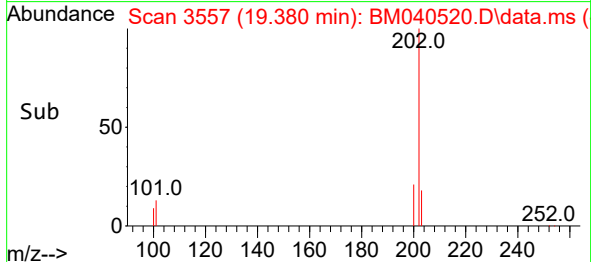

#20
Pyrene
Concen: 0.384 ng/ul
RT: 19.742 min Scan# 3635
Delta R.T. -0.005 min
Lab File: BM040520.D
Acq: 02 Jul 2023 02:04

Tgt Ion:202 Resp: 43903
Ion Ratio Lower Upper
202 100
101 16.4 12.6 18.8
100 13.9 9.8 14.6


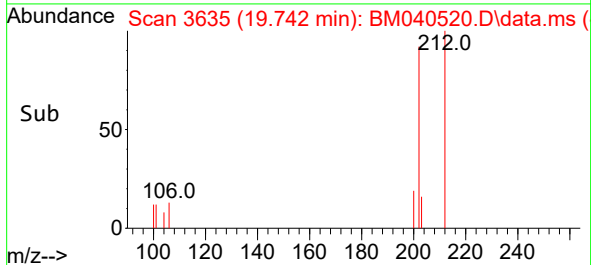

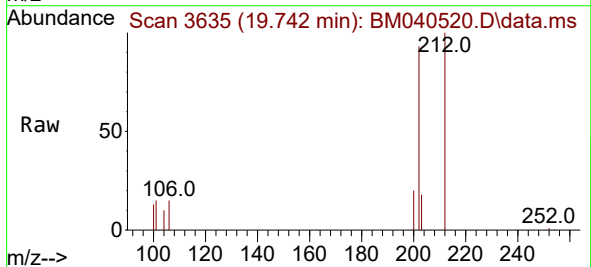


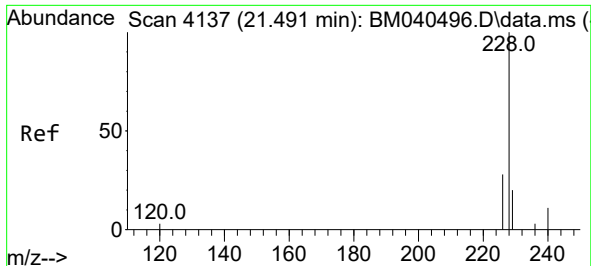

#21
Benzo(a)anthracene
Concen: 0.270 ng/ul
RT: 21.486 min Scan# 4135
Delta R.T. -0.006 min
Lab File: BM040520.D
Acq: 02 Jul 2023 02:04




Instrument :
BNA_M
ClientSampleId :
DCGB0


Tgt Ion:228 Resp: 22892
Ion Ratio Lower Upper
228 100
229 23.6 16.0 24.0
226 30.0 22.3 33.5

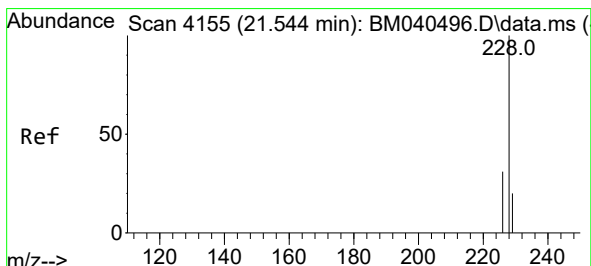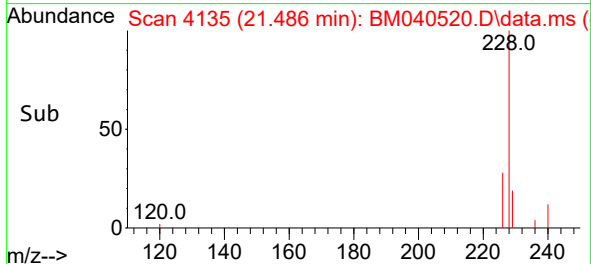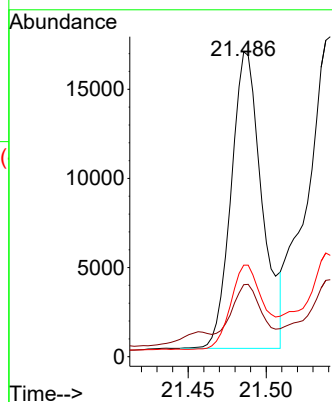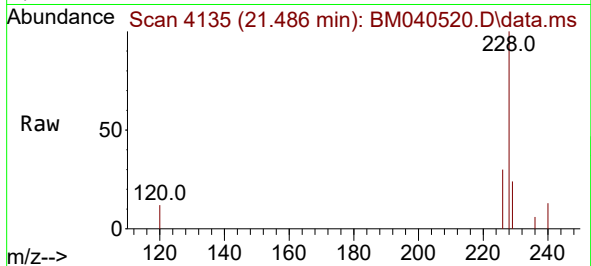

#22
Chrysene
Concen: 0.309 ng/ul
RT: 21.541 min Scan# 4154
Delta R.T. -0.003 min
Lab File: BM040520.D
Acq: 02 Jul 2023 02:04


Tgt Ion:228 Resp: 29964
Ion Ratio Lower Upper
228 100
226 31.7 24.9 37.3
229 24.1 15.8 23.6#

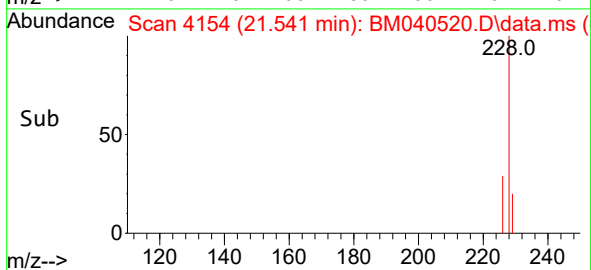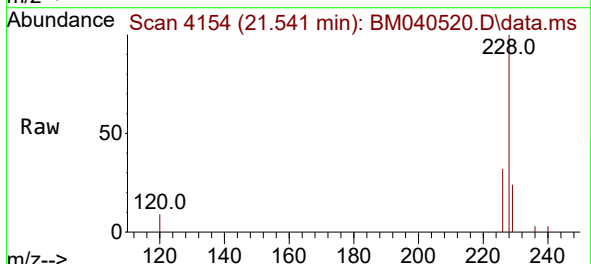


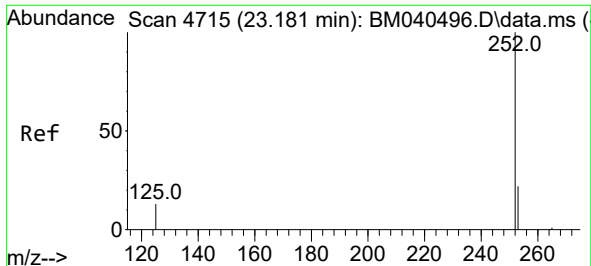


#24
Benzo(b)fluoranthene
Concen: 0.473 ng/ul
RT: 23.181 min Scan# 4715
Delta R.T. 0.000 min
Lab File: BM040520.D
Acq: 02 Jul 2023 02:04

Instrument :
BNA_M
ClientSampleId :
DCGB0







Tgt Ion:252 Resp: 42505
Ion Ratio Lower Upper
252 100
253 28.8 0.0 52.8
125 28.3 0.0 43.0



#26
Benzo(a)pyrene
Concen: 0.303 ng/ul
RT: 23.803 min Scan# 4928
Delta R.T. -0.009 min
Lab File: BM040520.D
Acq: 02 Jul 2023 02:04

Tgt Ion:252 Resp: 24520
Ion Ratio Lower Upper
252 100
253 32.0 22.9 34.3
125 35.7 21.0 31.4#

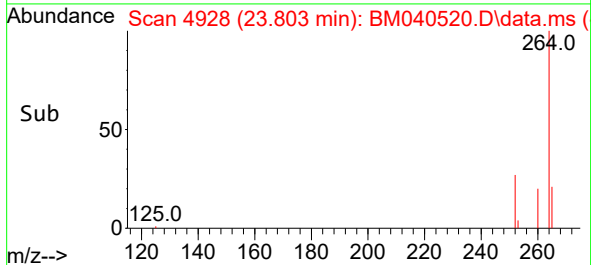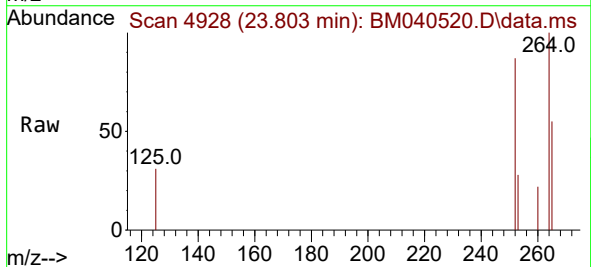



#27

Indeno(1,2,3-cd)pyrene

Concen: 0.210 ng/ul

RT: 26.417 min Scan# 5

Delta R.T. -0.003 min

Lab File: BM040520.D

Acq: 02 Jul 2023 02:04

Instrument :

BNA_M

ClientSampleId :

DCGB0





Tgt Ion:276 Resp: 23643

Ion Ratio Lower Upper

276 100

138 19.3 24.5 36.7#

227 0.0 0.1 0.1#

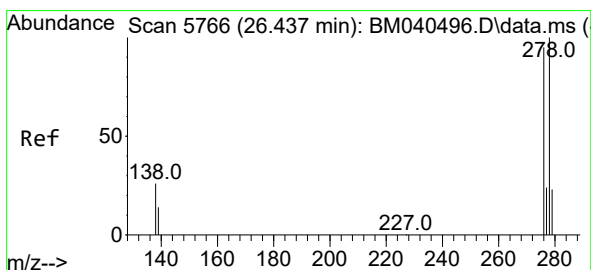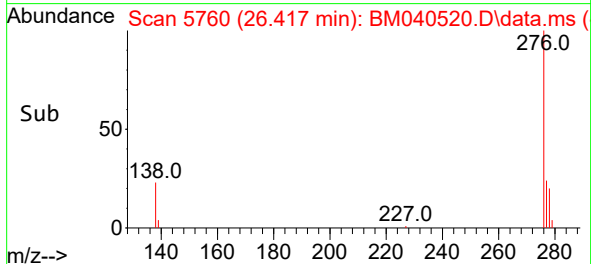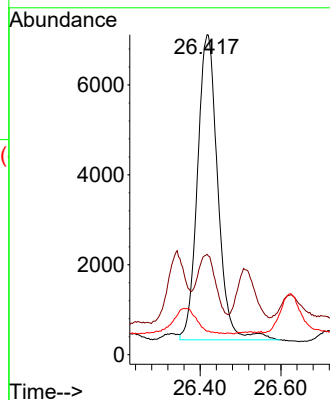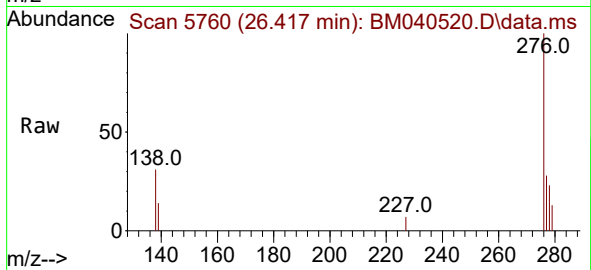

#28

Dibenzo(a,h)anthracene

Concen: 0.063 ng/ul

RT: 26.427 min Scan# 5763

Delta R.T. -0.010 min

Lab File: BM040520.D

Acq: 02 Jul 2023 02:04




Tgt Ion:278 Resp: 5577


Ion Ratio Lower Upper

278 100

139 53.6 17.9 26.9#


279 53.8 22.0 33.0#

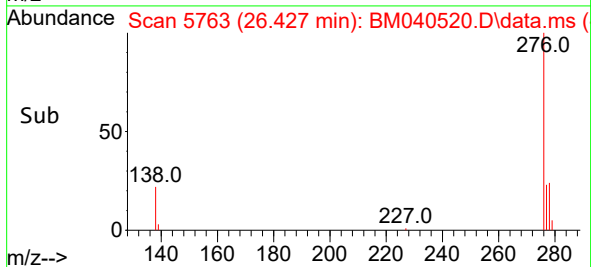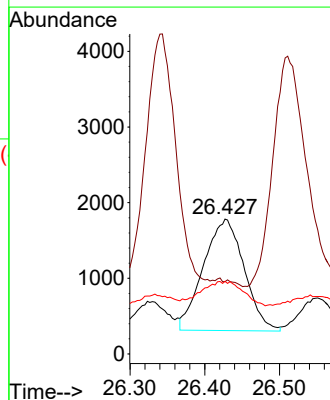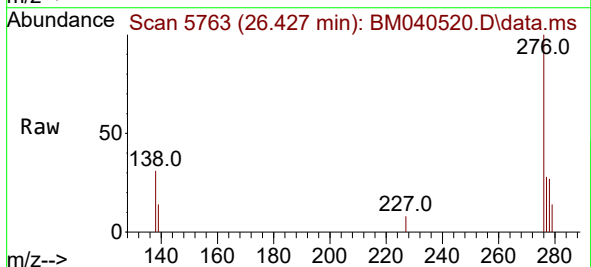



#29
Benzo(g,h,i)perylene
Concen: 0.227 ng/ul
RT: 27.195 min Scan# 51
Delta R.T. 0.010 min
Lab File: BM040520.D
Acq: 02 Jul 2023 02:04

Instrument :
BNA_M
ClientSampleId :
DCGB0

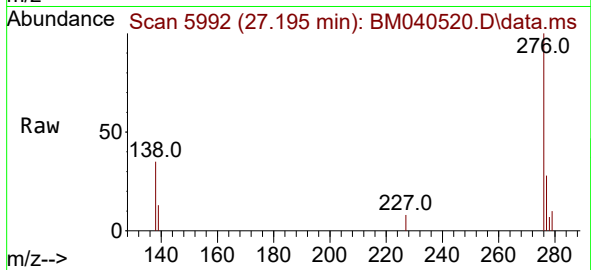

Tgt Ion:276 Resp: 22406
Ion Ratio Lower Upper
276 100
138 34.9 23.0 34.6#
277 28.1 20.3 30.5

