




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070123\
Data File : BM040510.D
Acq On : 01 Jul 2023 19:14
Operator : MA/JU
Sample : 03161-22DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCFX8DL

Manual IntegrationsAPPROVED

Quant Time: Jul 01 23:48:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 03:00:05 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/02/2023
Supervised By :Sohil Jodhani 07/02/2023

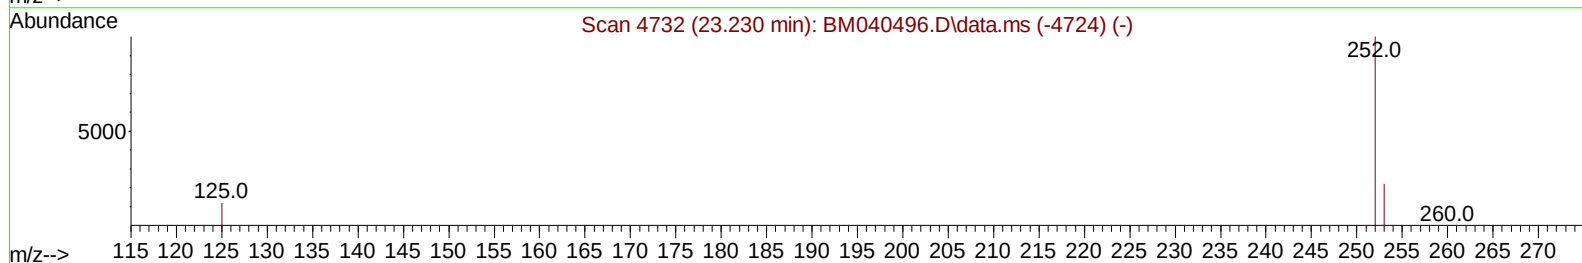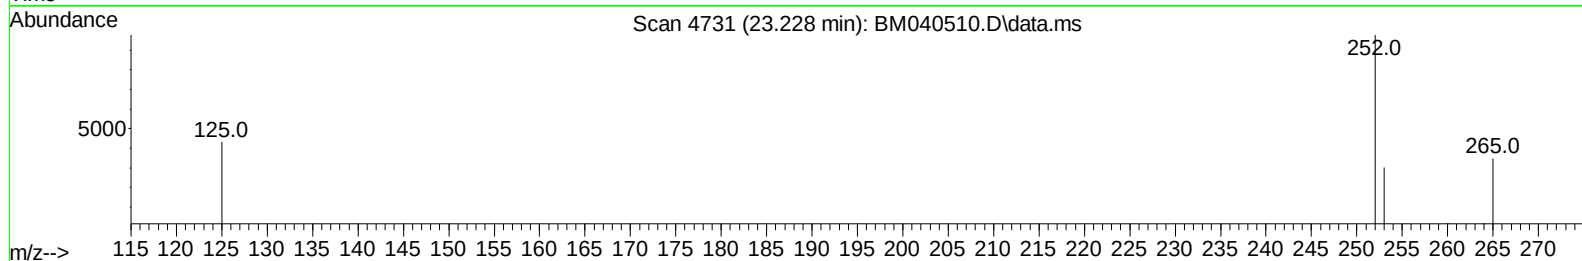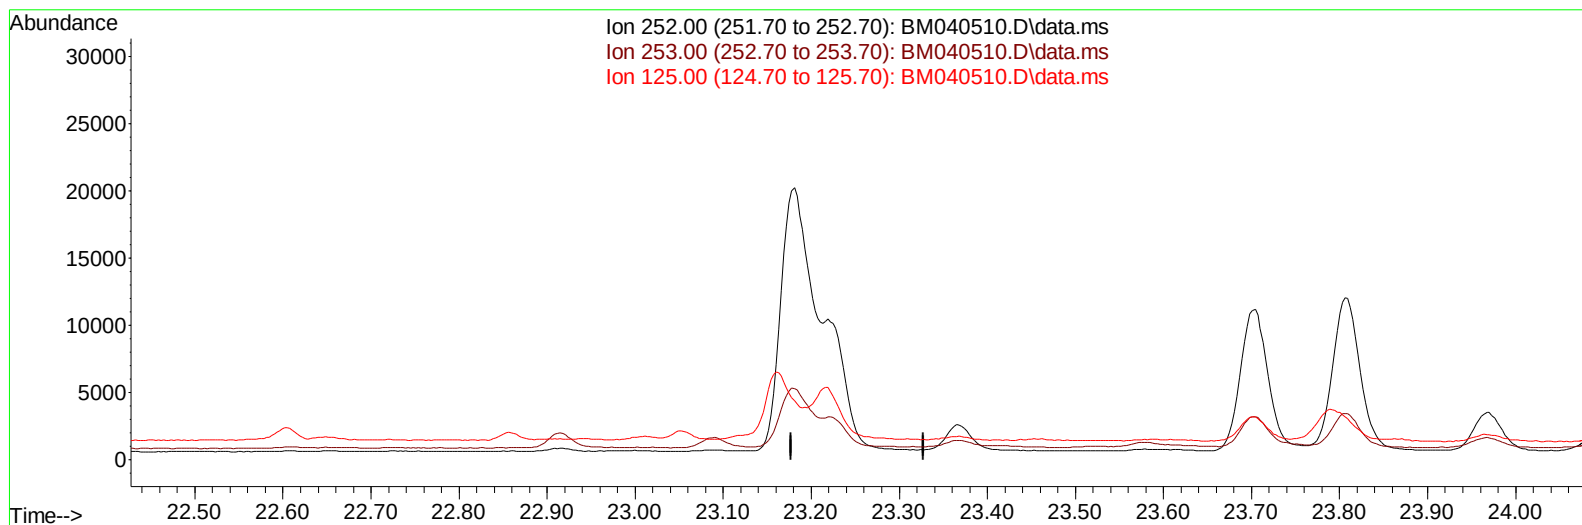

TIC: BM040510.D\data.ms

(25) Benzo(k)fluoranthene

23.227min (-23.227) 0.00 ng/u1

response 0

Ion	Exp%	Act%
252.00	100.00	0.00
253.00	26.50	0.00#
125.00	20.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070123\
 Data File : BM040510.D
 Acq On : 01 Jul 2023 19:14
 Operator : MA/JU
 Sample : 03161-22DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCFX8DL

Manual IntegrationsAPPROVED

Quant Time: Jul 01 23:48:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 03:00:05 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/02/2023
 Supervised By :Sohil Jodhani 07/02/2023

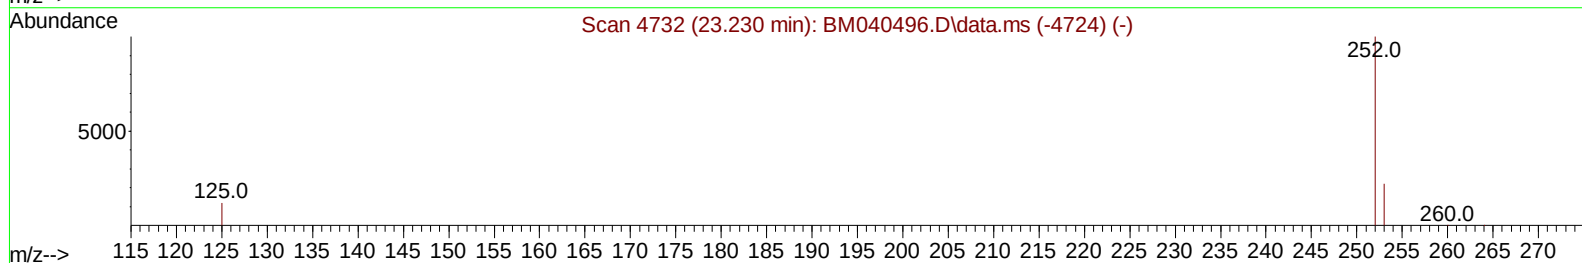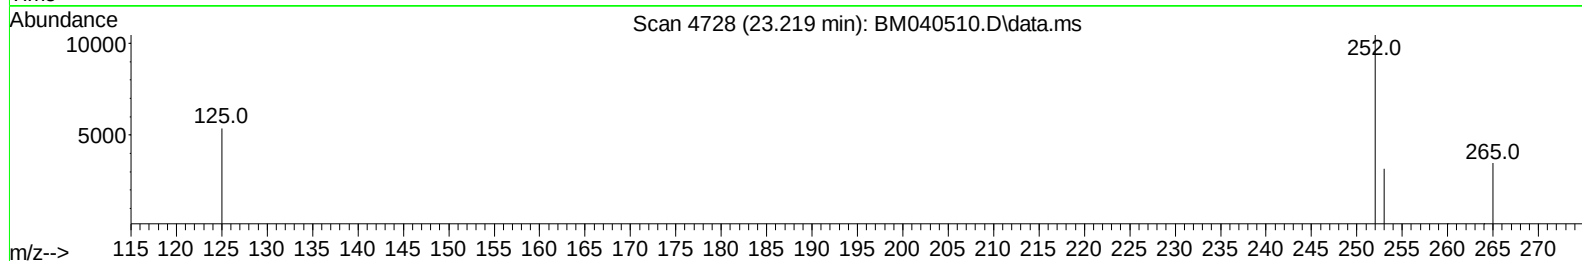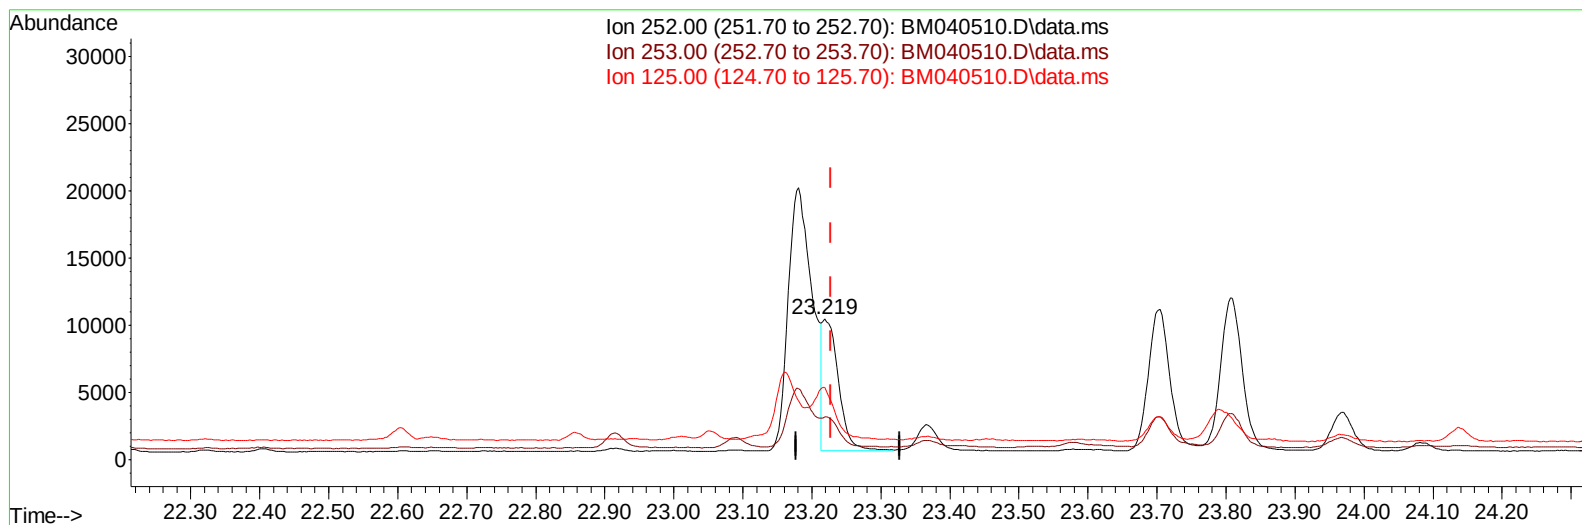

TIC: BM040510.D\data.ms

(25) Benzo(k)fluoranthene

23.219min (-0.009) 0.25 ng/ul m

response 15770

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	30.26
125.00	20.50	51.25#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070123\
 Data File : BM040510.D
 Acq On : 01 Jul 2023 19:14
 Operator : MA/JU
 Sample : 03161-22DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCFX8DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/02/2023
 Supervised By :Sohil Jodhani 07/02/2023

Quant Time: Jul 01 23:48:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 03:00:05 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.932	152		6959	0.400	ng/ul	0.00
4) Naphthalene-d8	10.740	136		25389	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.573	164		12453	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.324	188		25516	0.400	ng/ul	0.00
17) Chrysene-d12	21.503	240		18122	0.400	ng/ul	0.00
23) Perylene-d12	23.915	264		16621	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.325	96		4189	0.383	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.329	152		1211	0.034	ng/ul	0.00
18) Fluoranthene-d10	19.347	212		2187	0.038	ng/ul	0.00
Target Compounds							
						Qvalue	
7) 2-Methylnaphthalene	12.406	142		881	0.021	ng/ul	95
10) Acenaphthylene	14.295	152		1586	0.029	ng/ul#	77
15) Phenanthrene	17.362	178		16668	0.210	ng/ul	99
16) Anthracene	17.455	178		1918	0.029	ng/ul#	81
19) Fluoranthene	19.380	202		55870	0.726	ng/ul	98
20) Pyrene	19.742	202		45561	0.552	ng/ul	99
21) Benzo(a)anthracene	21.486	228		22919	0.374	ng/ul	97
22) Chrysene	21.541	228		31097	0.445	ng/ul	97
24) Benzo(b)fluoranthene	23.181	252		47635	0.741	ng/ul	100
25) Benzo(k)fluoranthene	23.219	252		15770m	0.249	ng/ul	
26) Benzo(a)pyrene	23.806	252		24824	0.428	ng/ul	100
27) Indeno(1,2,3-cd)pyrene	26.417	276		23801	0.295	ng/ul#	84
28) Dibenzo(a,h)anthracene	26.420	278		5796	0.092	ng/ul#	67
29) Benzo(g,h,i)perylene	27.188	276		21476	0.304	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070123\
Data File : BM040510.D
Acq On : 01 Jul 2023 19:14
Operator : MA/JU
Sample : 03161-22DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCFX8DL

Manual IntegrationsAPPROVED

Quant Time: Jul 01 23:48:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 03:00:05 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/02/2023
Supervised By :Sohil Jodhani 07/02/2023

