

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070219\
 Data File : BM021350.D
 Acq On : 02 Jul 2019 19:24
 Operator : HP/JU
 Sample : PB121053BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK53

Quant Time: Jul 03 01:13:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:09:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	205191	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	898484	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	550987	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1075132	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	894044	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1059307	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	14388	3.33	ng/uL	0.00
5) Phenol-d5	6.92	99	371292	20.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	222917	20.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	314845	21.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	327641	21.98	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	168481	23.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	198679	24.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	376099	22.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	57742	3.36	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	1198702	24.08	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	1400801	22.99	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	112125	13.85	ng/ul	0.00
57) Fluorene-d10	15.39	176	976159	22.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	94061	14.23	ng/ul	0.00
70) Anthracene-d10	17.24	188	1318423	23.60	ng/ul	0.00
78) Pyrene-d10	19.54	212	1312918	24.47	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	1510973	24.18	ng/ul	0.00

Target Compounds


					Qvalue	
6) Phenol	6.95	94	24854	1.471	ng/ul#	92
44) Dimethylphthalate	13.85	163	383698	8.466	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070219\
Data File : BM021350.D
Acq On : 02 Jul 2019 19:24
Operator : HP/JU
Sample : PB121053BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK53

Quant Time: Jul 03 01:13:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:09:29 2019
Response via : Initial Calibration

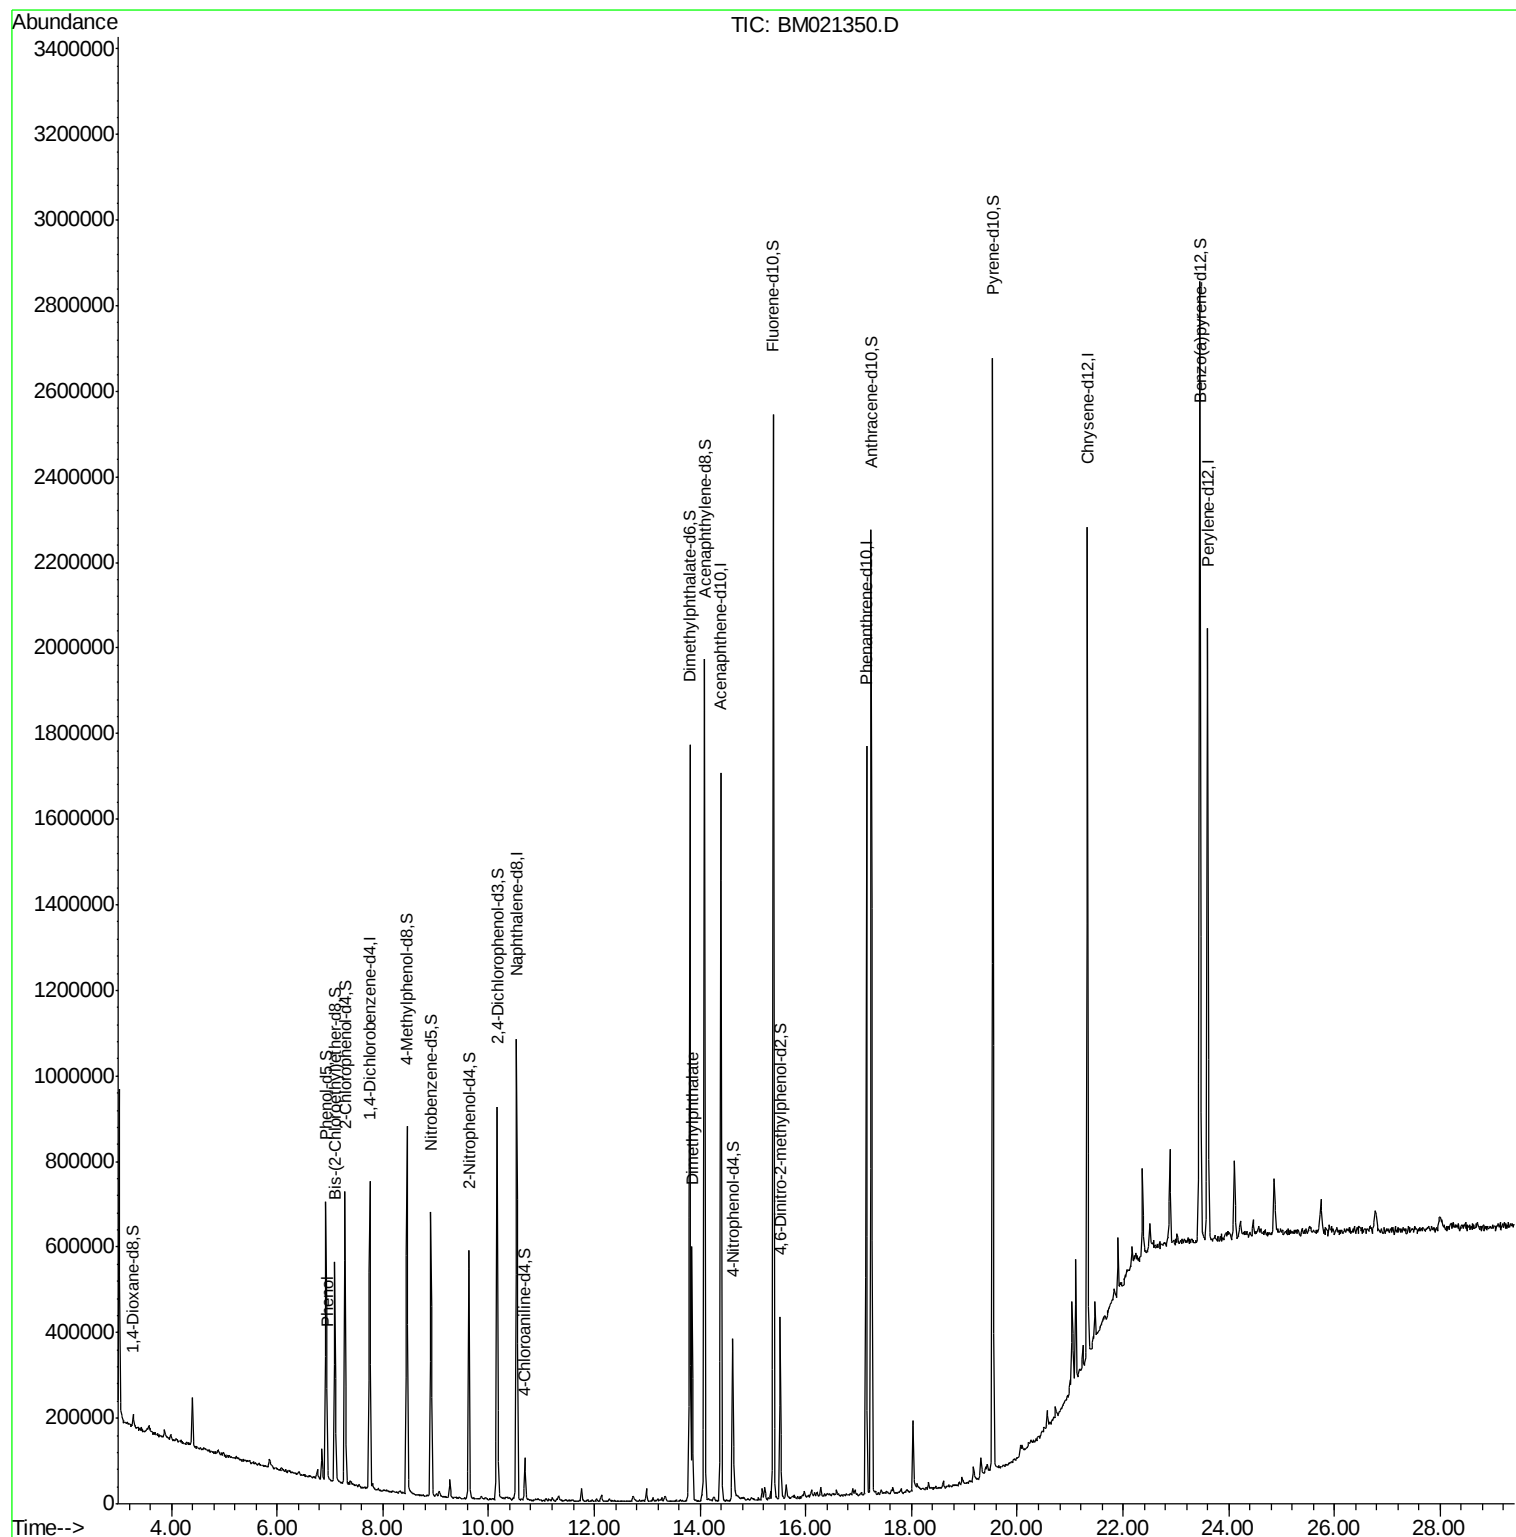

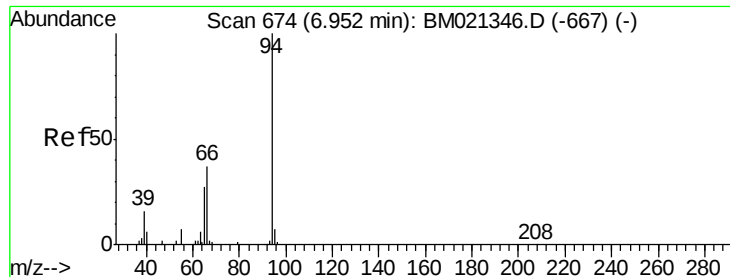

#6

Phenol

Concen: 1.471 ng/ul

RT: 6.95 min Scan# 673

Delta R.T. -0.01 min

Lab File: BM021350.D

Acq: 02 Jul 2019 19:24

Instrument :

BNA_M

ClientSampleId :

SBLK53


Tgt Ion: 94 Resp: 24854

Ion Ratio Lower Upper

94 100

65 28.7 22.6 34.0

66 47.0 31.2 46.8#



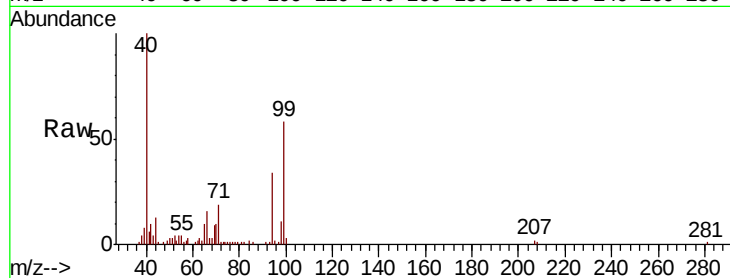


Abundance

Ion 94.00 (93.70 to 94.70): BM021346.D (-667) (-)

Ion 65.00 (64.70 to 65.70): BM021346.D (-667) (-)

Ion 66.00 (65.70 to 66.70): BM021346.D (-667) (-)

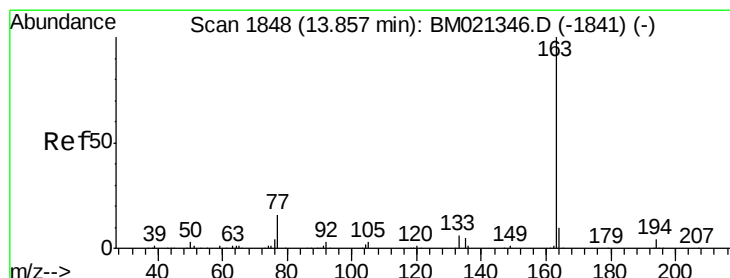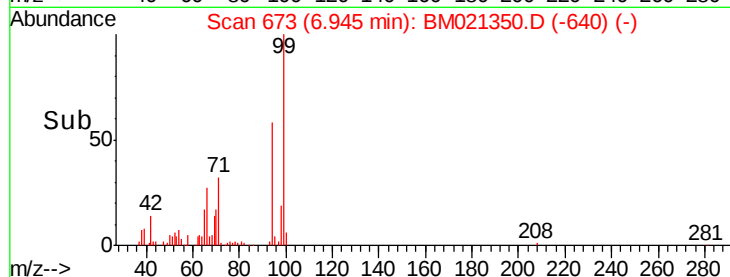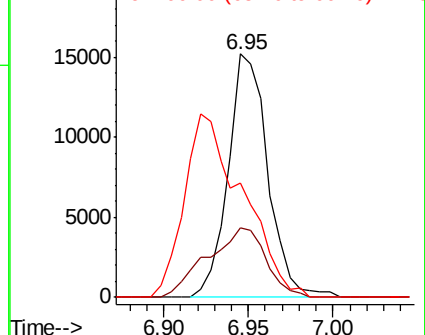

#44

Dimethylphthalate

Concen: 8.466 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BM021350.D

Acq: 02 Jul 2019 19:24


Tgt Ion: 163 Resp: 383698

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 10.1 7.7 11.5

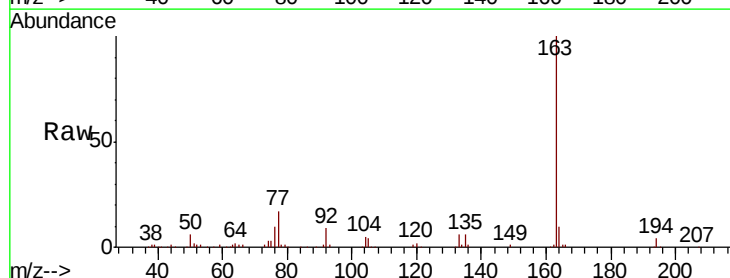

Abundance

Ion 163.00 (162.70 to 163.70): BM021346.D (-1841) (-)

Ion 194.00 (193.70 to 194.70): BM021346.D (-1841) (-)

Ion 164.00 (163.70 to 164.70): BM021346.D (-1841) (-)

