

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070219\
 Data File : BM021353.D
 Acq On : 02 Jul 2019 21:13
 Operator : HP/JU
 Sample : K3578-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJF2

Quant Time: Jul 03 01:13:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:09:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	214684	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	964240	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	608950	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1246708	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	967431	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1130592	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	14865	3.29	ng/uL	0.00
5) Phenol-d5	6.92	99	352564	18.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	203000	18.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	297364	19.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	313158	20.08	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	160199	20.46	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	182812	21.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	358090	20.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	389442	21.13	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	1106588	20.11	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	1289771	19.15	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	95246	10.64	ng/ul	0.00
57) Fluorene-d10	15.39	176	932555	19.48	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	77537	10.12	ng/ul	0.00
70) Anthracene-d10	17.24	188	1270267	19.61	ng/ul	0.00
78) Pyrene-d10	19.54	212	1206647	20.79	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.45	264	1266706	18.99	ng/ul	0.00


Target Compounds					Qvalue	
44) Dimethylphthalate	13.85	163	386425	7.715	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070219\
Data File : BM021353.D
Acq On : 02 Jul 2019 21:13
Operator : HP/JU
Sample : K3578-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJF2

Quant Time: Jul 03 01:13:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:09:29 2019
Response via : Initial Calibration

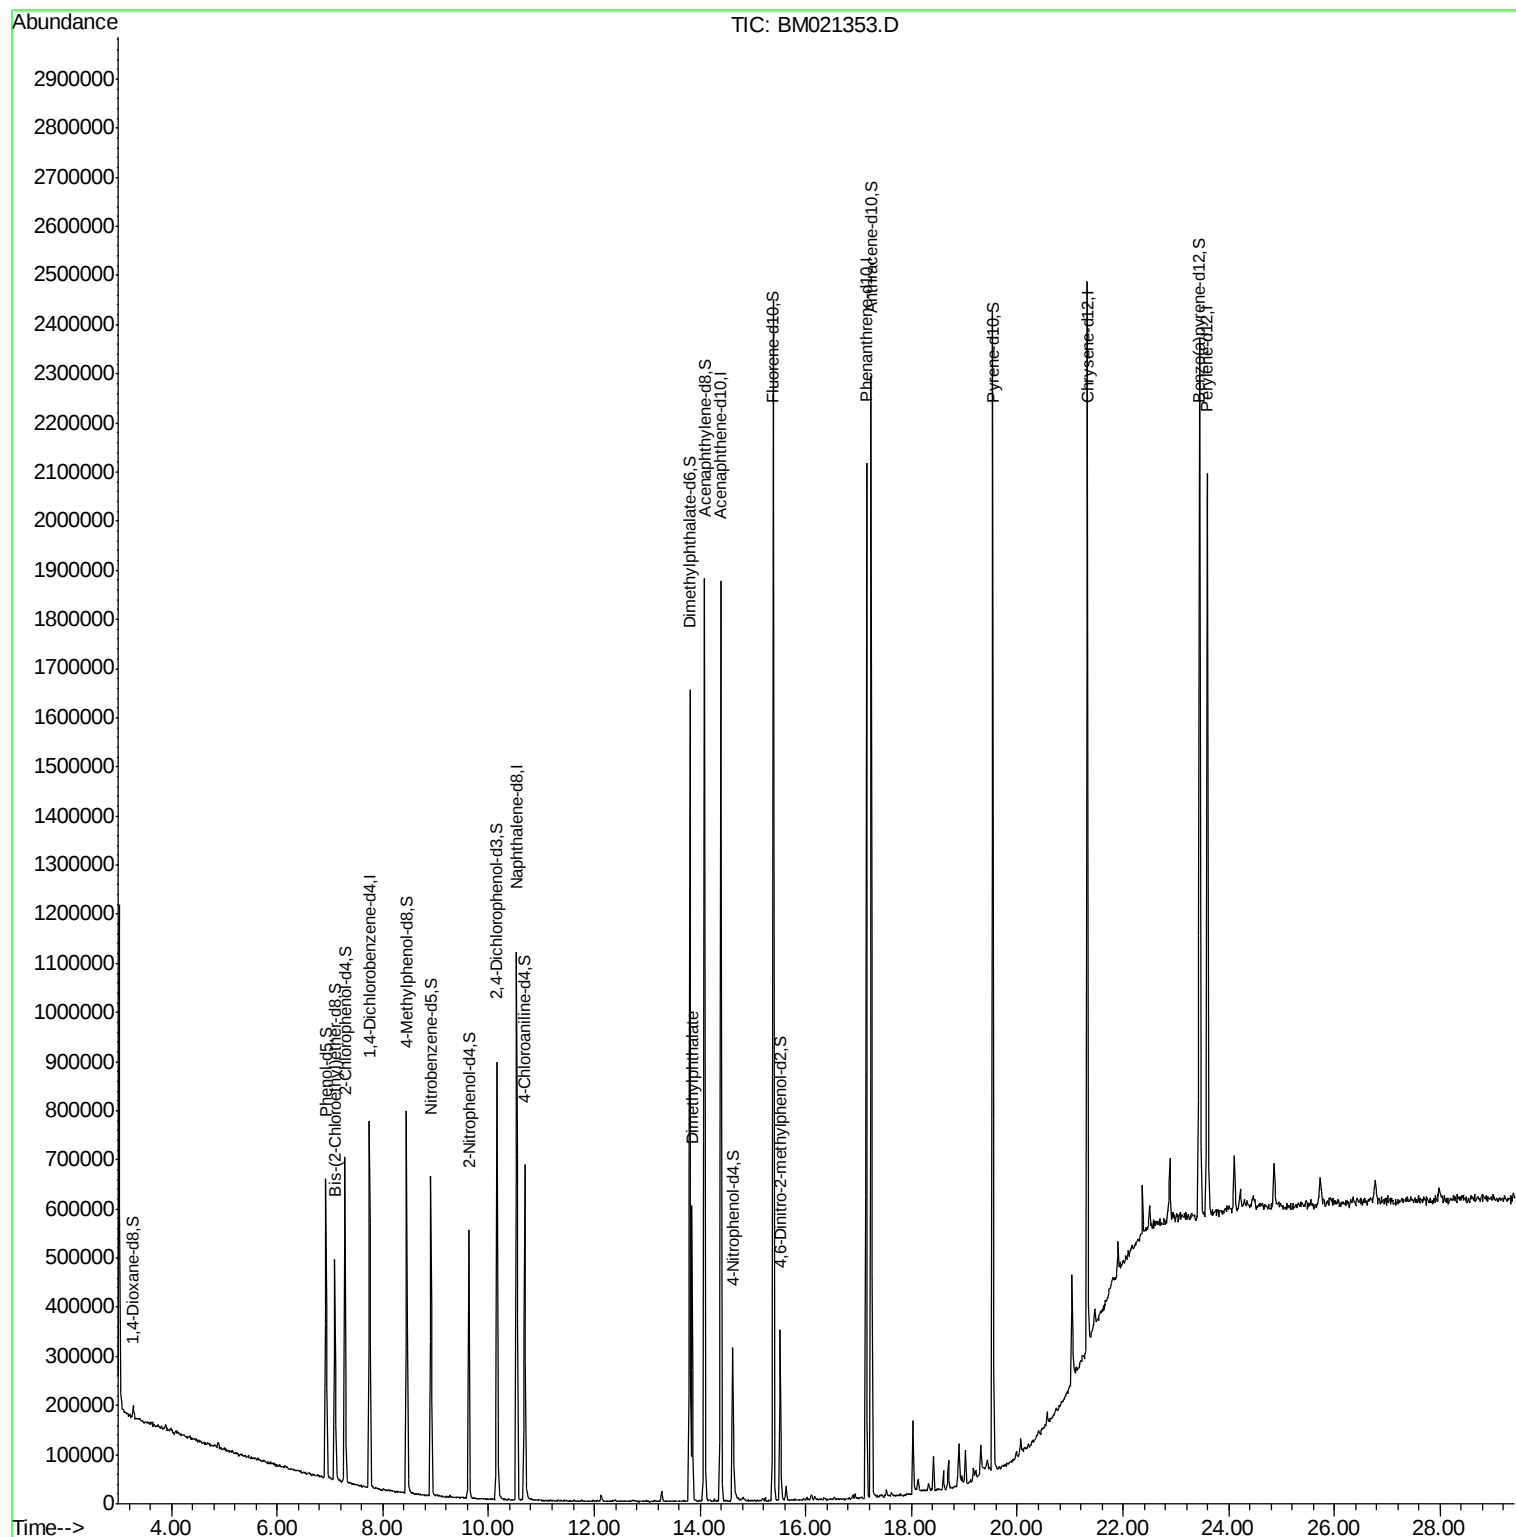

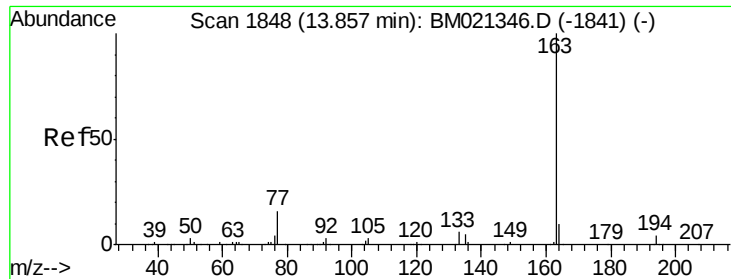

#44
 Dimethylphthalate
 Concen: 7.715 ng/ul
 RT: 13.85 min Scan# 1847
 Delta R.T. -0.01 min
 Lab File: BM021353.D
 Acq: 02 Jul 2019 21:13

Instrument :
 BNA_M
 ClientSampleId :
 JLJF2

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.4	5.2
164	10.3	7.7	11.5

