

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070219\
 Data File : BM021356.D
 Acq On : 02 Jul 2019 23:03
 Operator : HP/JU
 Sample : K3578-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJF8

Quant Time: Jul 03 01:13:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:09:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	229079	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	1034498	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	657468	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1386621	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	1089101	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1235250	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	20606	4.27	ng/uL	0.00
5) Phenol-d5	6.92	99	487771	24.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	279600	23.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	408393	25.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	429180	25.79	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	219913	26.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	254164	27.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	491354	25.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	603259	30.50	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	1551902	26.12	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	1791709	24.64	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	163163	16.88	ng/ul	0.00
57) Fluorene-d10	15.39	176	1322589	25.59	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	144211	16.92	ng/ul	0.00
70) Anthracene-d10	17.24	188	1865981	25.90	ng/ul	0.00
78) Pyrene-d10	19.54	212	1792460	27.43	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.45	264	1855152	25.46	ng/ul	0.00


Target Compounds					Qvalue	
44) Dimethylphthalate	13.85	163	520434	9.624	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070219\
Data File : BM021356.D
Acq On : 02 Jul 2019 23:03
Operator : HP/JU
Sample : K3578-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJF8

Quant Time: Jul 03 01:13:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:09:29 2019
Response via : Initial Calibration

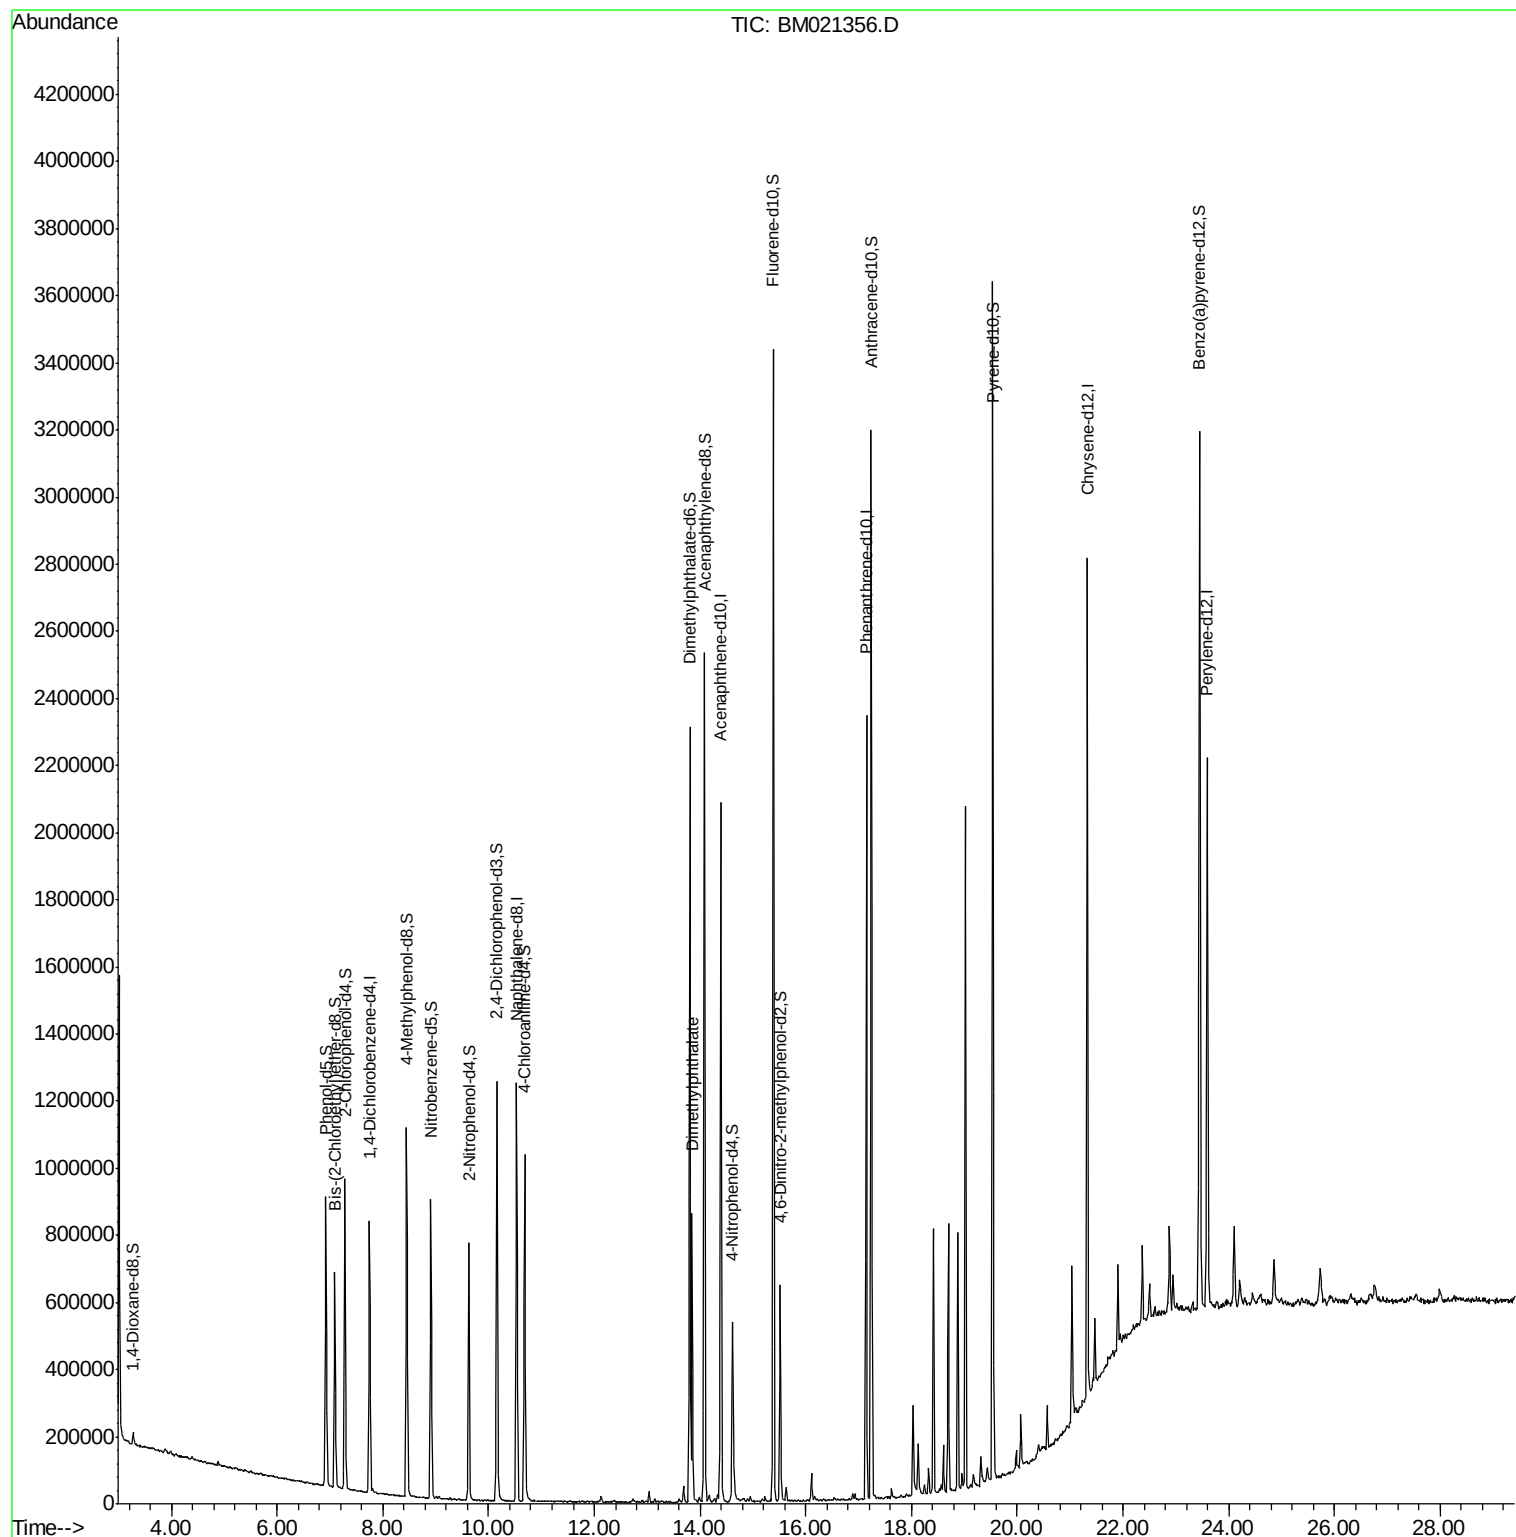

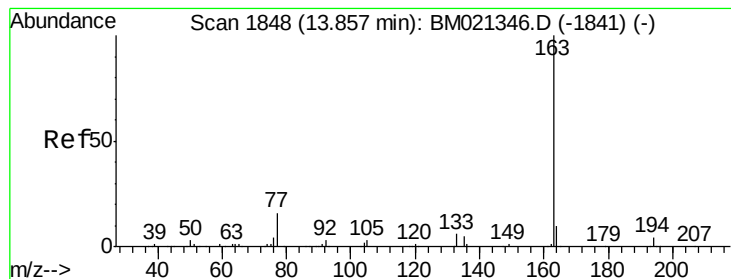

#44

Dimethylphthalate

Concen: 9.624 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BM021356.D

Acq: 02 Jul 2019 23:03

Instrument :

BNA_M

ClientSampleId :

JLJF8


Tgt Ion:163 Resp: 520434

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 10.6 7.7 11.5

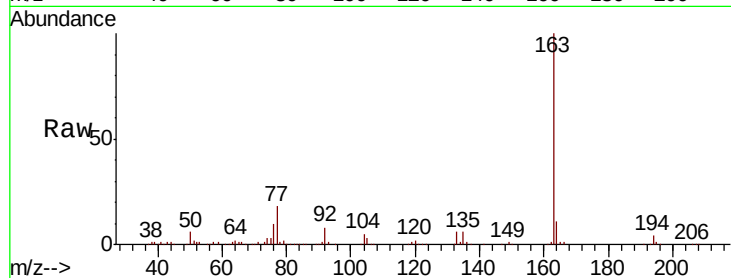

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

