

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070219\
 Data File : BM021357.D
 Acq On : 02 Jul 2019 23:39
 Operator : HP/JU
 Sample : K3578-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJG1

Quant Time: Jul 03 01:13:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:09:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	227771	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	1005132	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	621429	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1259186	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	1072499	20.00	ng/ul	0.00
85) Perylene-d12	23.59	264	1228542	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.28	96	4908	1.02	ng/uL	0.00
5) Phenol-d5	6.92	99	146717	7.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	88579	7.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	119405	7.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	134488	8.13	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	68399	8.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	75961	8.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	151890	8.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	153223	7.97	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	522099	9.30	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	576883	8.39	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	35087	3.84	ng/ul	0.00
57) Fluorene-d10	15.39	176	430265	8.81	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	29086	3.76	ng/ul	0.00
70) Anthracene-d10	17.24	188	610665	9.33	ng/ul	0.00
78) Pyrene-d10	19.53	212	640623	9.95	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.45	264	686700	9.47	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.85	163	163725	3.203	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070219\
Data File : BM021357.D
Acq On : 02 Jul 2019 23:39
Operator : HP/JU
Sample : K3578-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJG1

Quant Time: Jul 03 01:13:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:09:29 2019
Response via : Initial Calibration

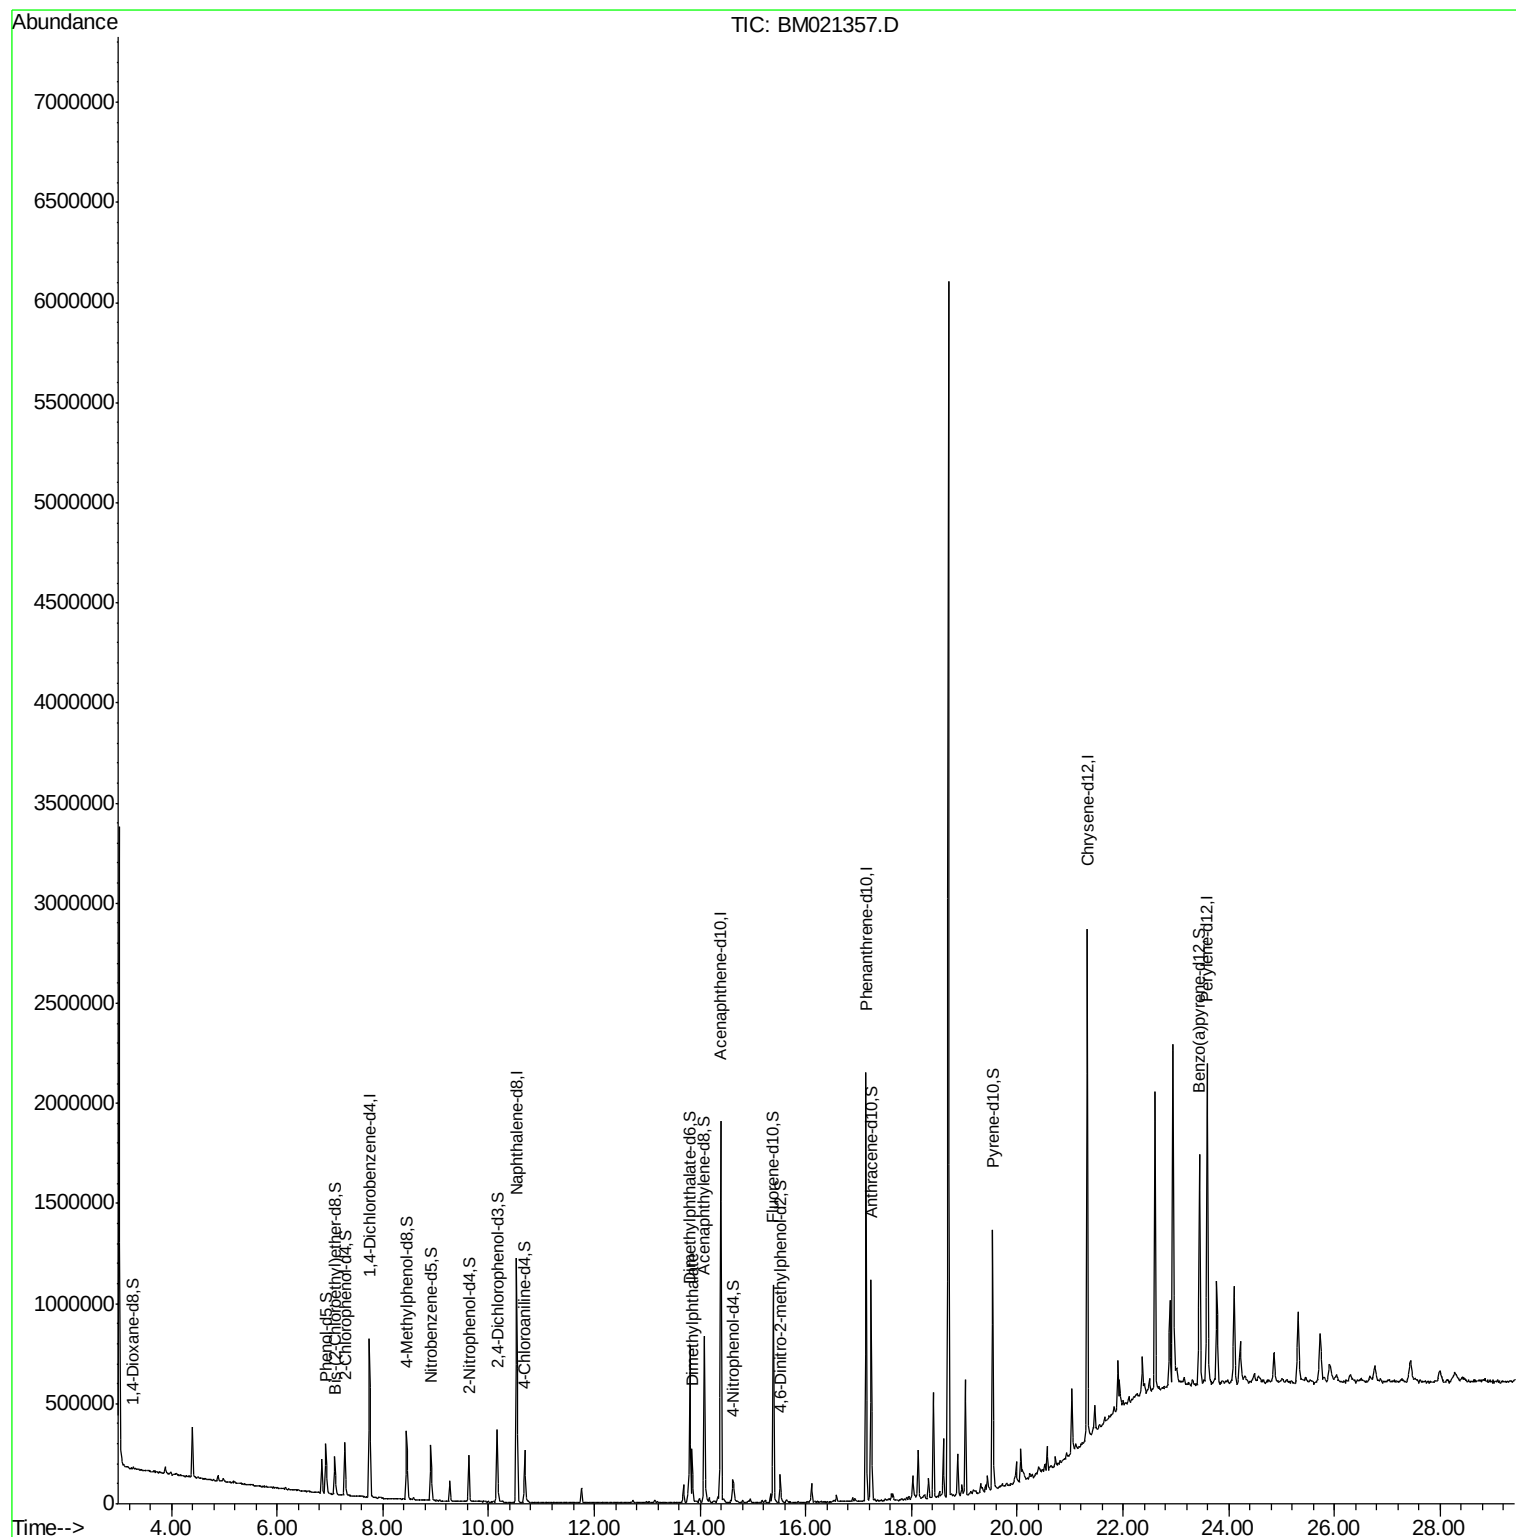

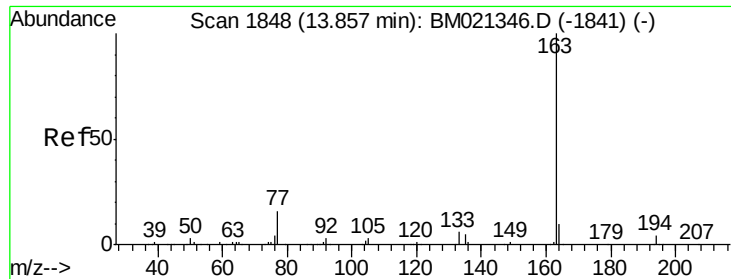

#44

Dimethylphthalate

Concen: 3.203 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BM021357.D

Acq: 02 Jul 2019 23:39

Instrument :

BNA_M

ClientSampleId :

JLJG1


Tgt Ion:163 Resp: 163725

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 10.8 7.7 11.5

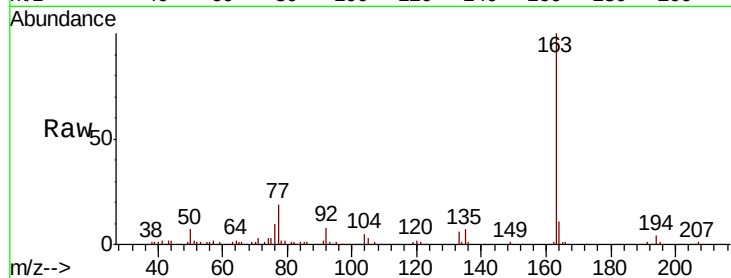

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

