

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070219\
 Data File : BM021351.D
 Acq On : 02 Jul 2019 20:01
 Operator : HP/JU
 Sample : K3497-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GAM06

Quant Time: Jul 03 01:13:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:09:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	214041	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	950411	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	589281	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1220975	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	956032	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1116869	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	10567	2.34	ng/uL	0.00
5) Phenol-d5	6.92	99	247053	13.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	145250	13.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	209754	13.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	200295	12.88	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	112988	14.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	128167	14.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	250479	14.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	271927	14.97	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	820413	15.41	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	933446	14.32	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	71504	8.26	ng/ul	0.00
57) Fluorene-d10	15.39	176	691104	14.92	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	60149	8.01	ng/ul	0.00
70) Anthracene-d10	17.24	188	993555	15.66	ng/ul	0.00
78) Pyrene-d10	19.54	212	1035525	18.05	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.45	264	1095285	16.62	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.85	163	283608	5.851	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070219\
Data File : BM021351.D
Acq On : 02 Jul 2019 20:01
Operator : HP/JU
Sample : K3497-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GAM06

Quant Time: Jul 03 01:13:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:09:29 2019
Response via : Initial Calibration

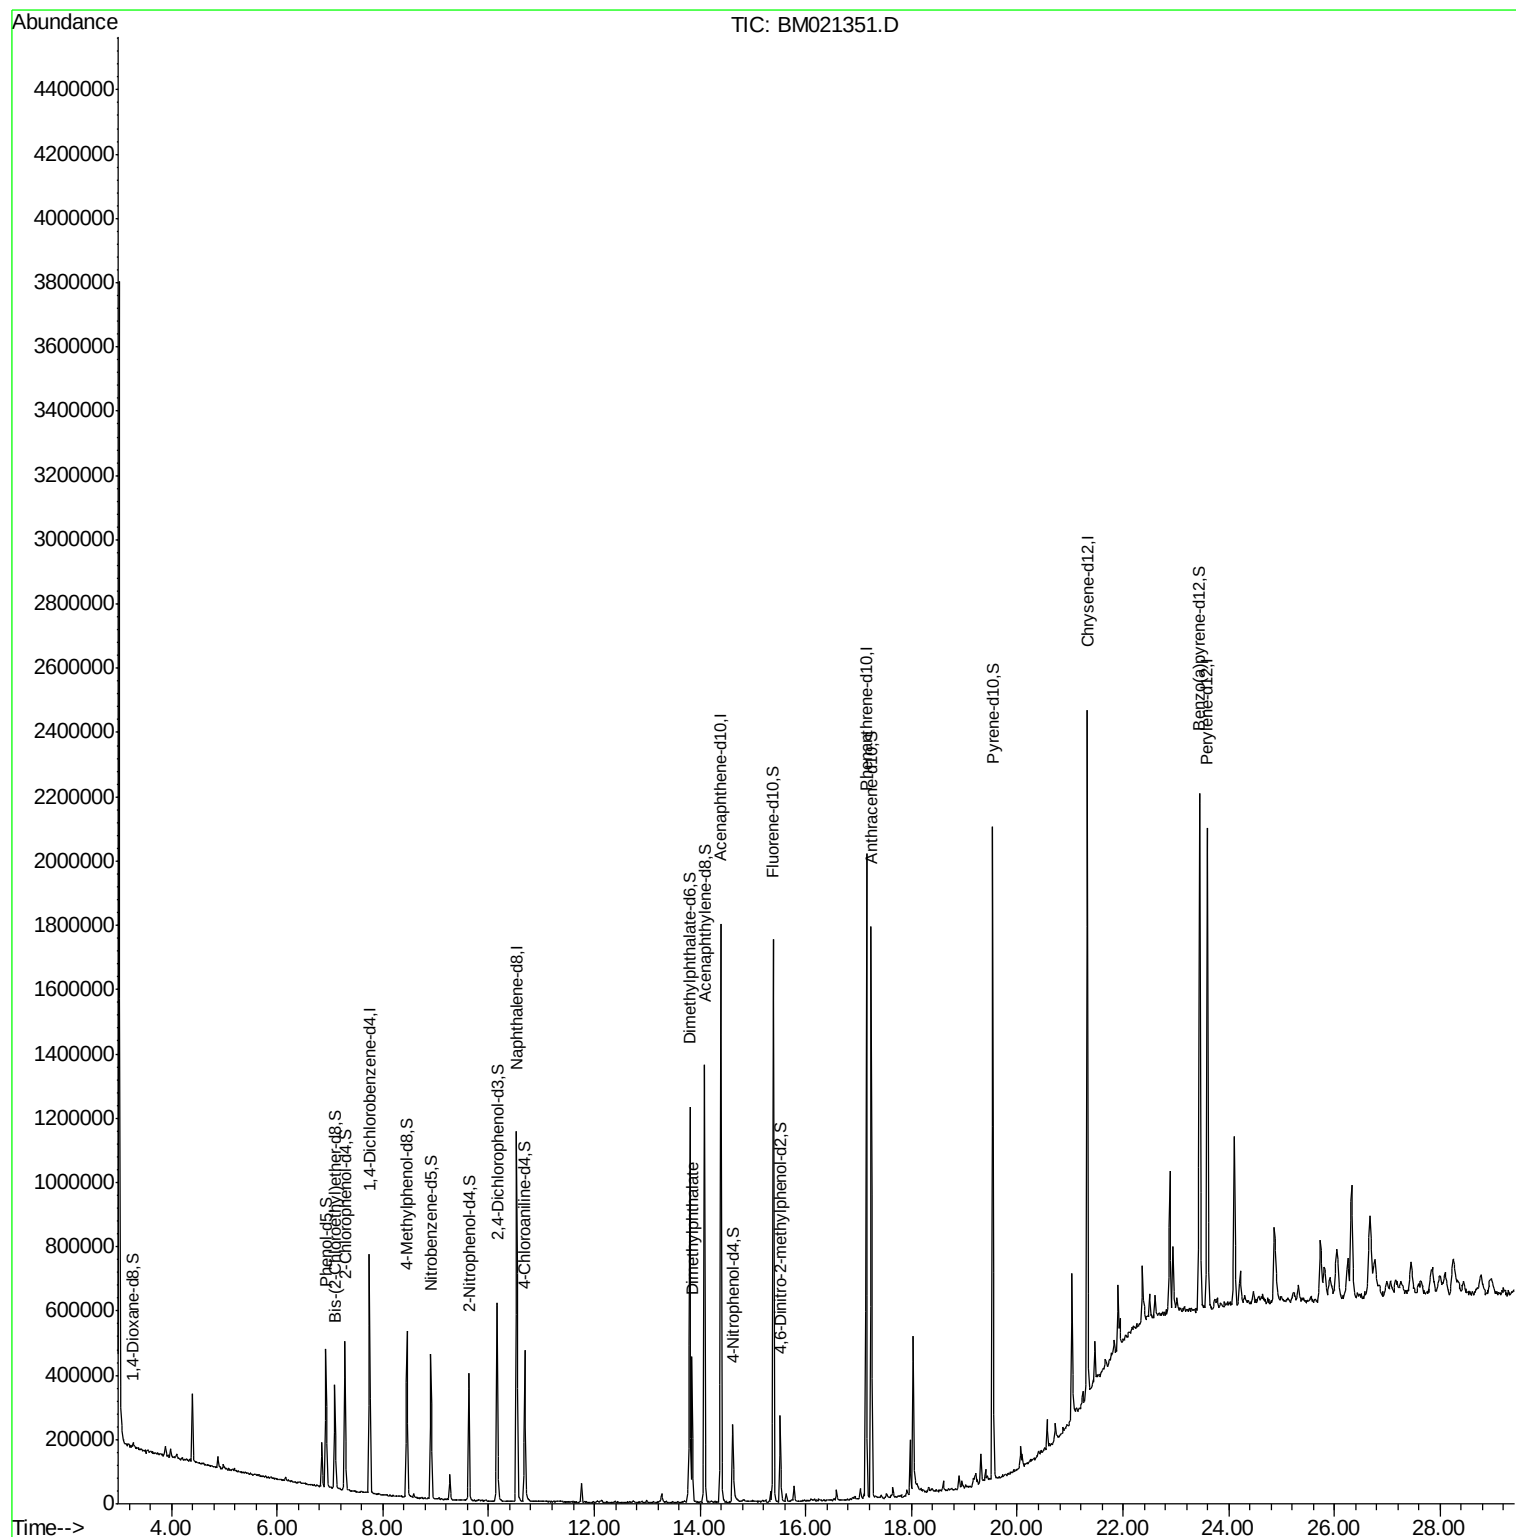

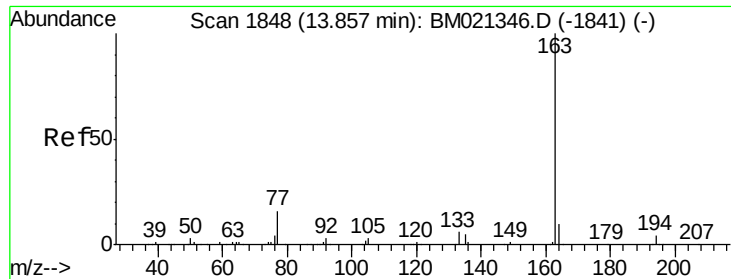

#44

Dimethylphthalate

Concen: 5.851 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BM021351.D

Acq: 02 Jul 2019 20:01

Instrument :

BNA_M

ClientSampleId :

GAM06


Tot Ion:163 Resp: 283608

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2

164 10.1 7.7 11.5

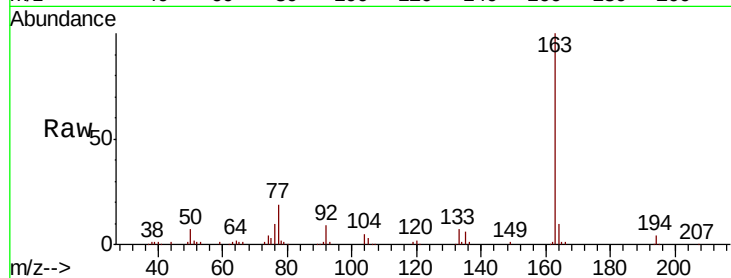

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

