

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070219\
 Data File : BM021355.D
 Acq On : 02 Jul 2019 22:26
 Operator : HP/JU
 Sample : K3578-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJF7

Quant Time: Jul 03 01:13:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:09:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	223486	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	1001620	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	642406	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1361410	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	1059532	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1204648	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	19569	4.16	ng/uL	0.00
5) Phenol-d5	6.92	99	462169	23.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	262220	22.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	386120	24.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	404208	24.89	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	208346	25.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	244784	27.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	470430	25.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	582165	30.40	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	1471773	25.36	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	1707072	24.02	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	135528	14.35	ng/ul	0.00
57) Fluorene-d10	15.39	176	1245577	24.67	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	121600	14.53	ng/ul	0.00
70) Anthracene-d10	17.24	188	1755563	24.81	ng/ul	0.00
78) Pyrene-d10	19.54	212	1676297	26.37	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	1726727	24.30	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.85	163	544584	10.306	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070219\
Data File : BM021355.D
Acq On : 02 Jul 2019 22:26
Operator : HP/JU
Sample : K3578-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJF7

Quant Time: Jul 03 01:13:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:09:29 2019
Response via : Initial Calibration

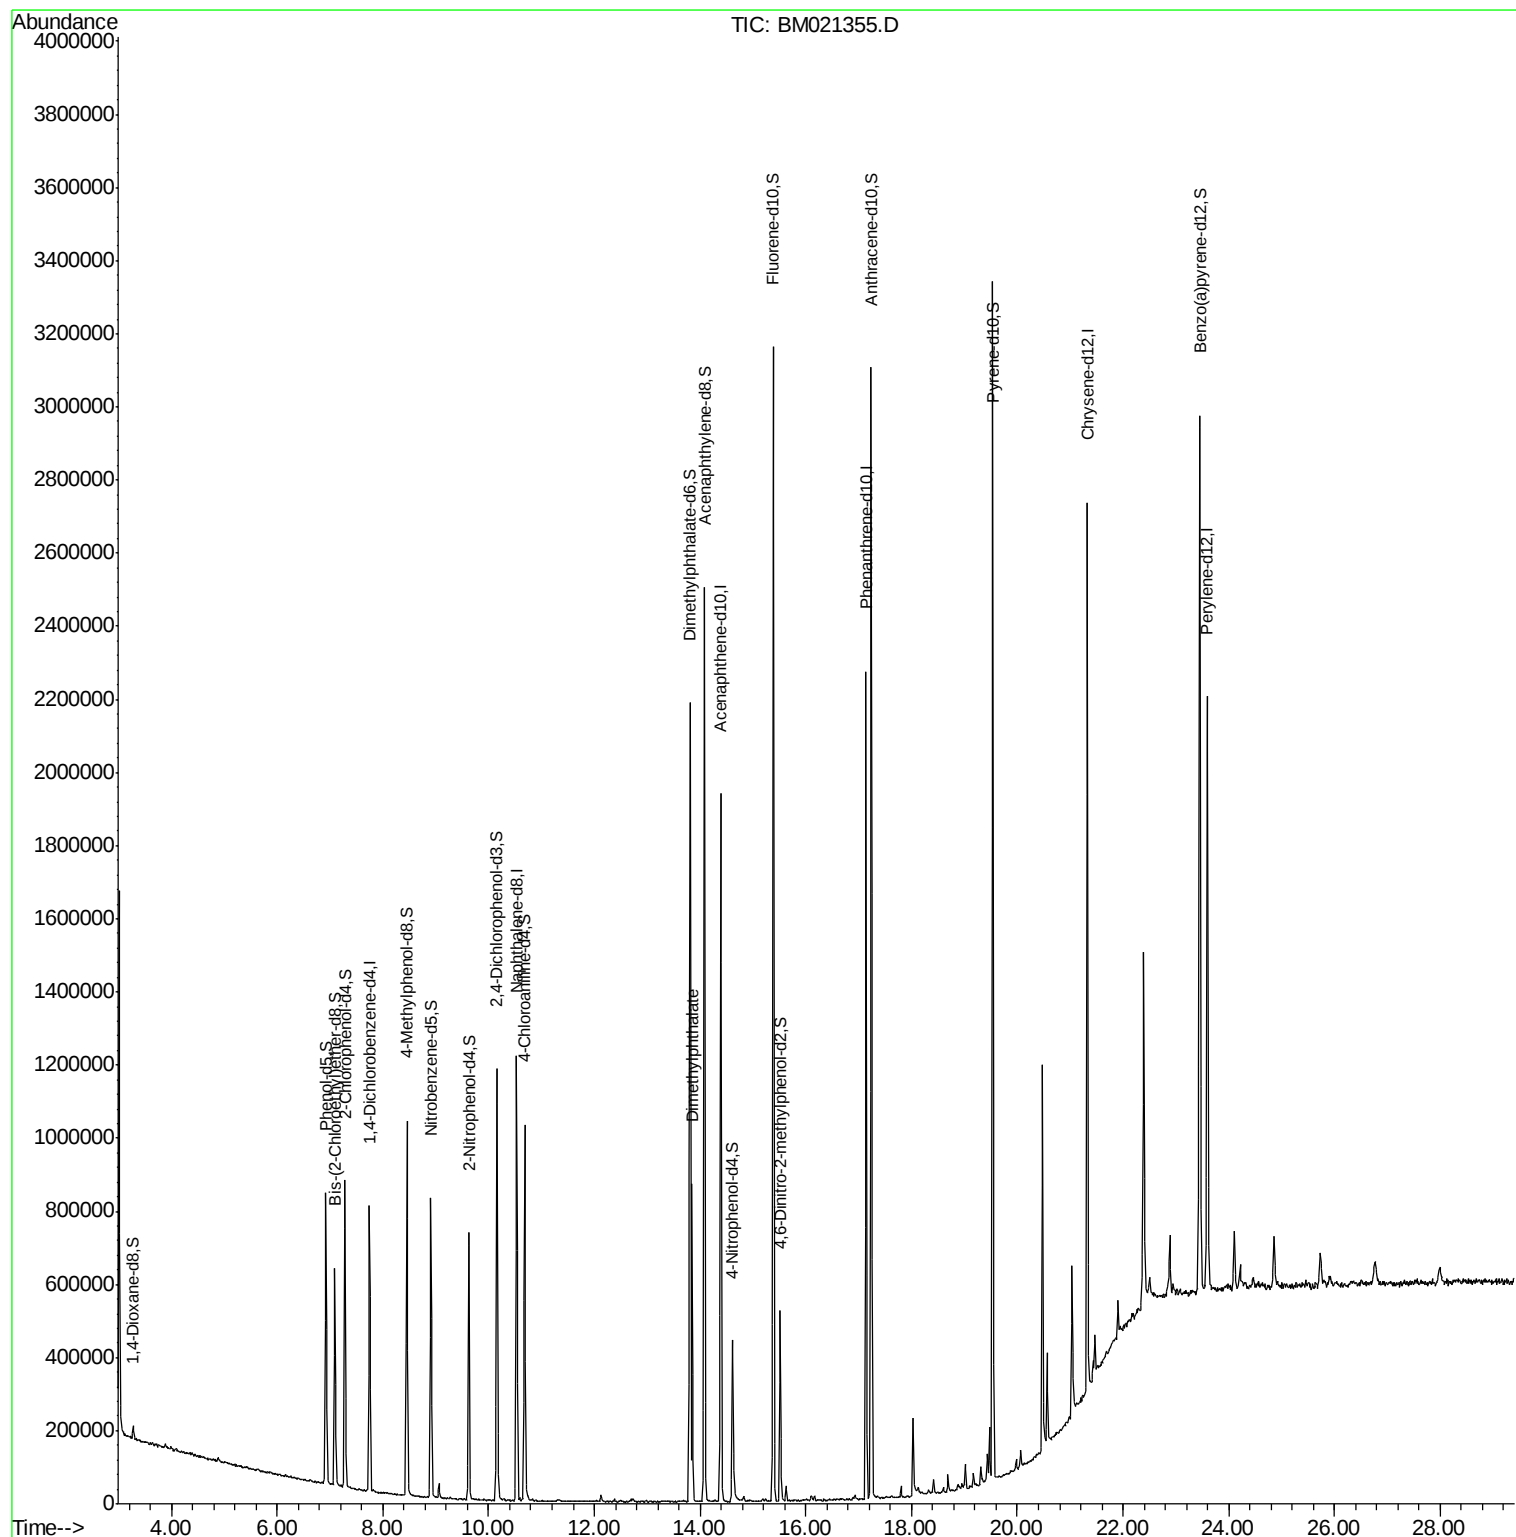

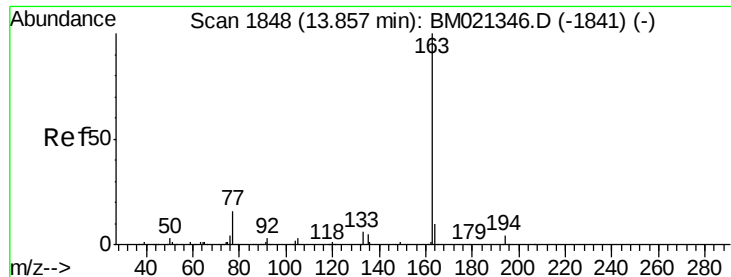

#44

Dimethylphthalate

Concen: 10.306 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BM021355.D

Acq: 02 Jul 2019 22:26

Instrument :

BNA_M

ClientSampleId :

JLJF7



Tot Ion:163 Resp: 544584

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 10.0 7.7 11.5

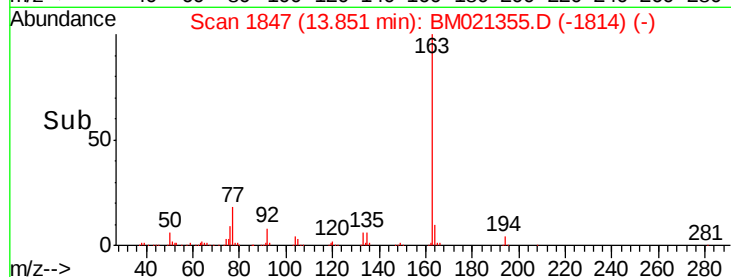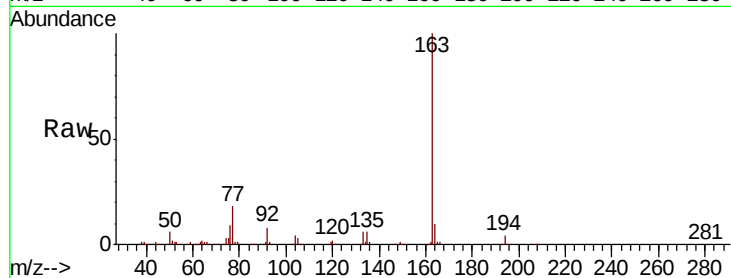

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

