

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
 Data File : BM021378.D
 Acq On : 03 Jul 2019 22:36
 Operator : HP/JU
 Sample : K3596-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 03 23:35:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:58:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	217583	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	942444	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	534721	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1024428	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	895289	20.00	ng/ul	0.00
85) Perylene-d12	23.59	264	1067192	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.28	96	24157	5.27	ng/uL	0.00
5) Phenol-d5	6.92	99	136739	7.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	320614	28.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	391786	25.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	259624	16.42	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	245455	32.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	279897	32.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	503532	29.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	68017	3.78	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	1589653	32.90	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	1858578	31.42	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	25278	3.22	ng/ul	0.01
57) Fluorene-d10	15.39	176	1298862	30.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	137608	21.85	ng/ul	0.00
70) Anthracene-d10	17.24	188	1756433	32.99	ng/ul	0.00
78) Pyrene-d10	19.53	212	1802120	33.54	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.45	264	2121834	33.70	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.85	163	76045	1.729	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021378.D
Acq On : 03 Jul 2019 22:36
Operator : HP/JU
Sample : K3596-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 03 23:35:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:58:18 2019
Response via : Initial Calibration

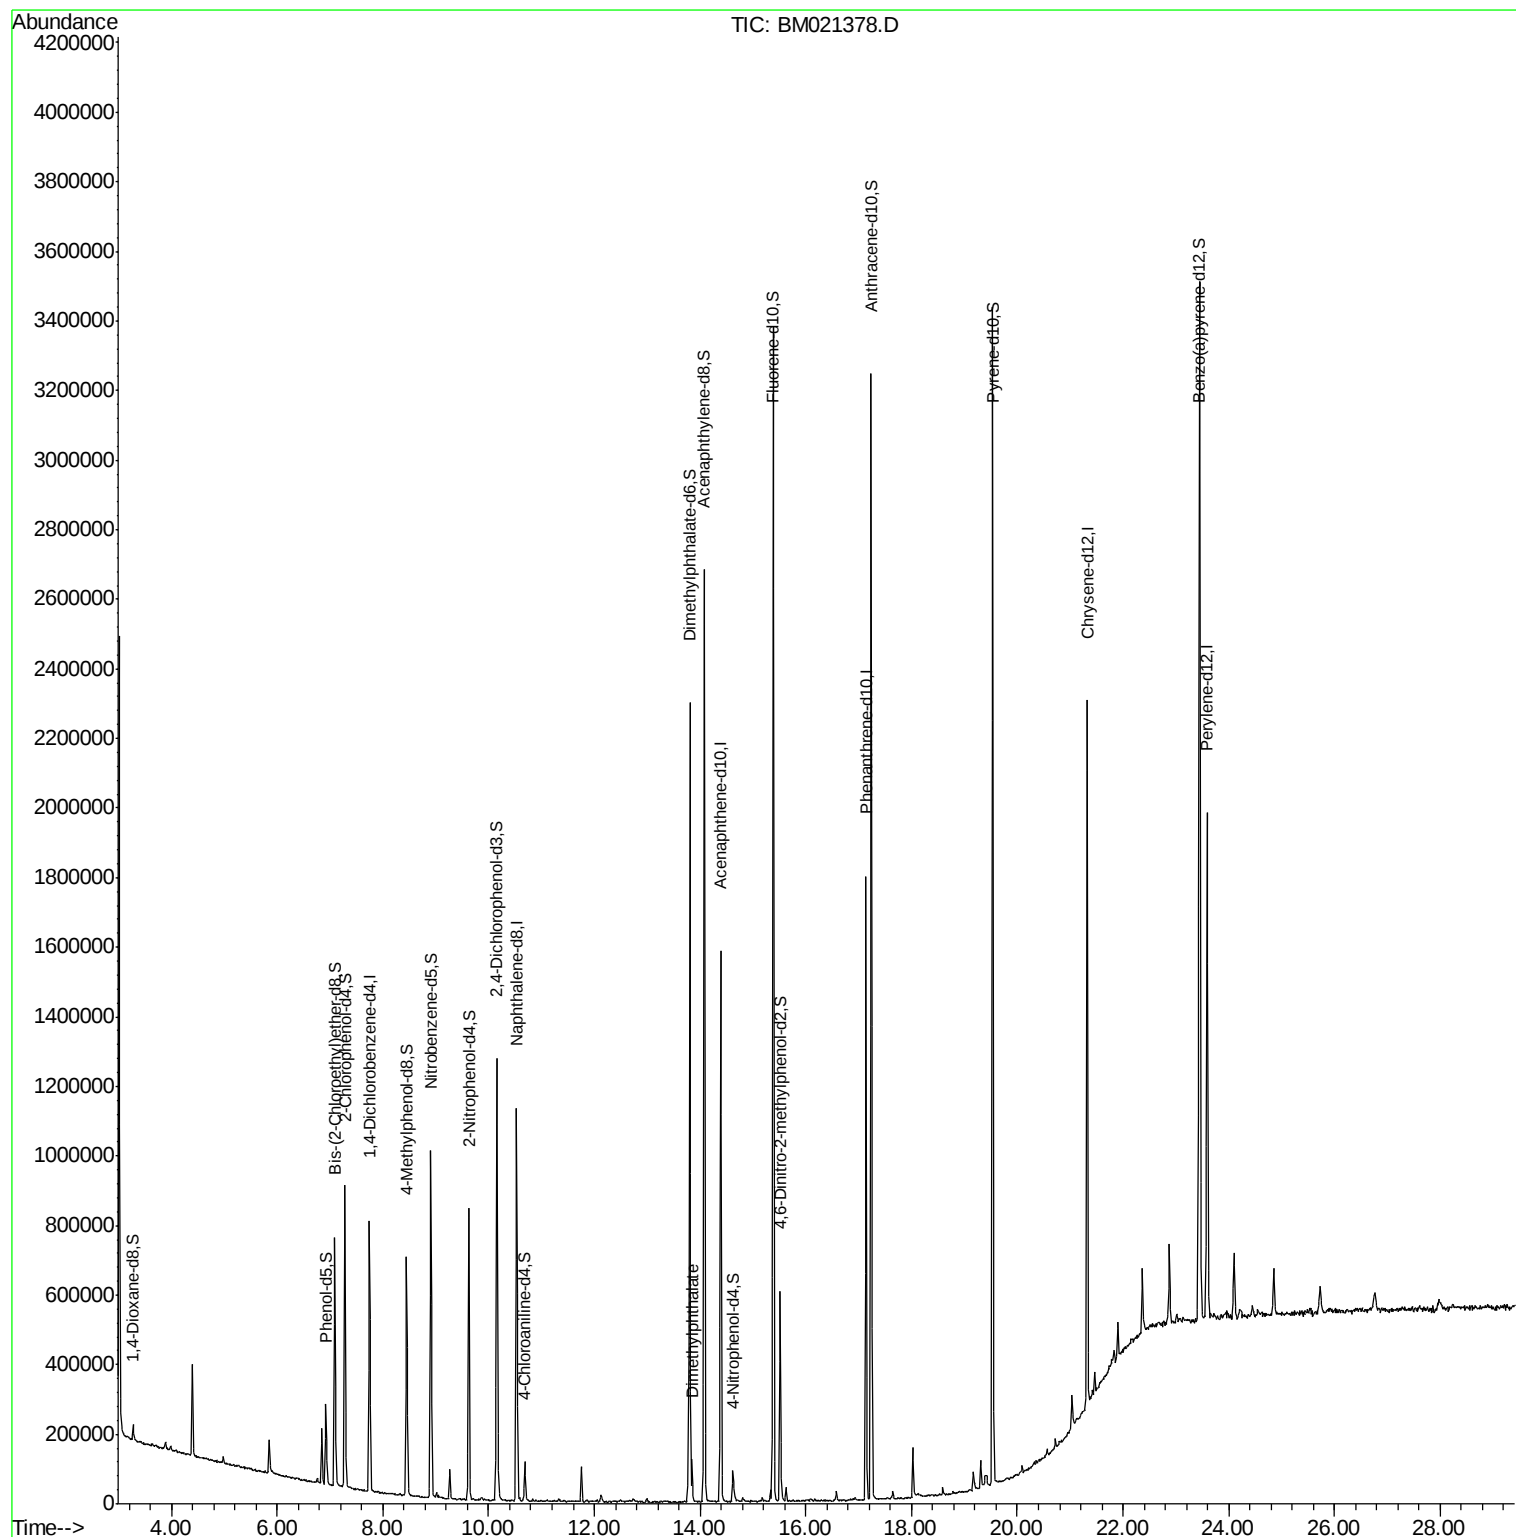

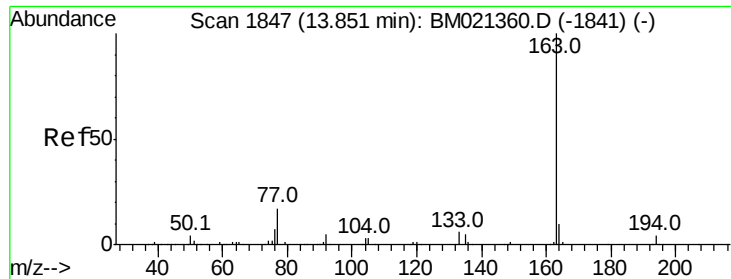

#44

Dimethylphthalate

Concen: 1.729 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. 0.00 min

Lab File: BM021378.D

Acq: 03 Jul 2019 22:36

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 76045

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 10.8 7.7 11.5

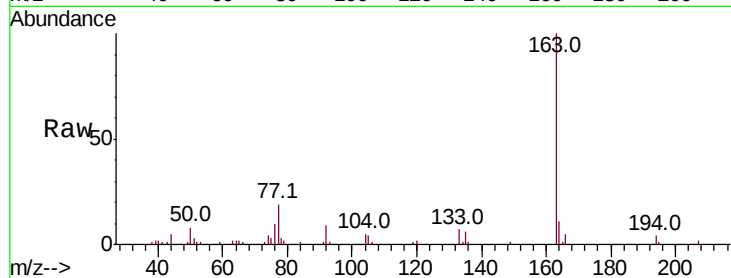

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

