
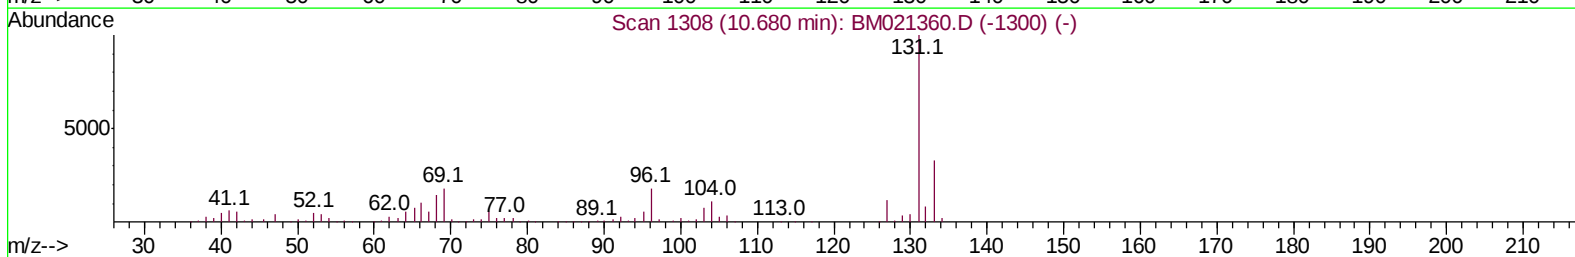
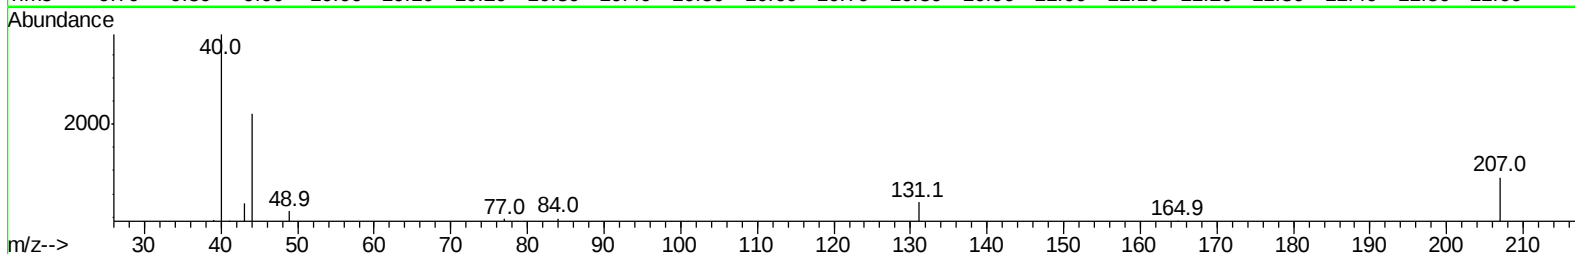


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021382.D
Acq On : 04 Jul 2019 01:05
Operator : HP/JU
Sample : K3462-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jul 04 01:56:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:58:18 2019
Response via : Initial Calibration

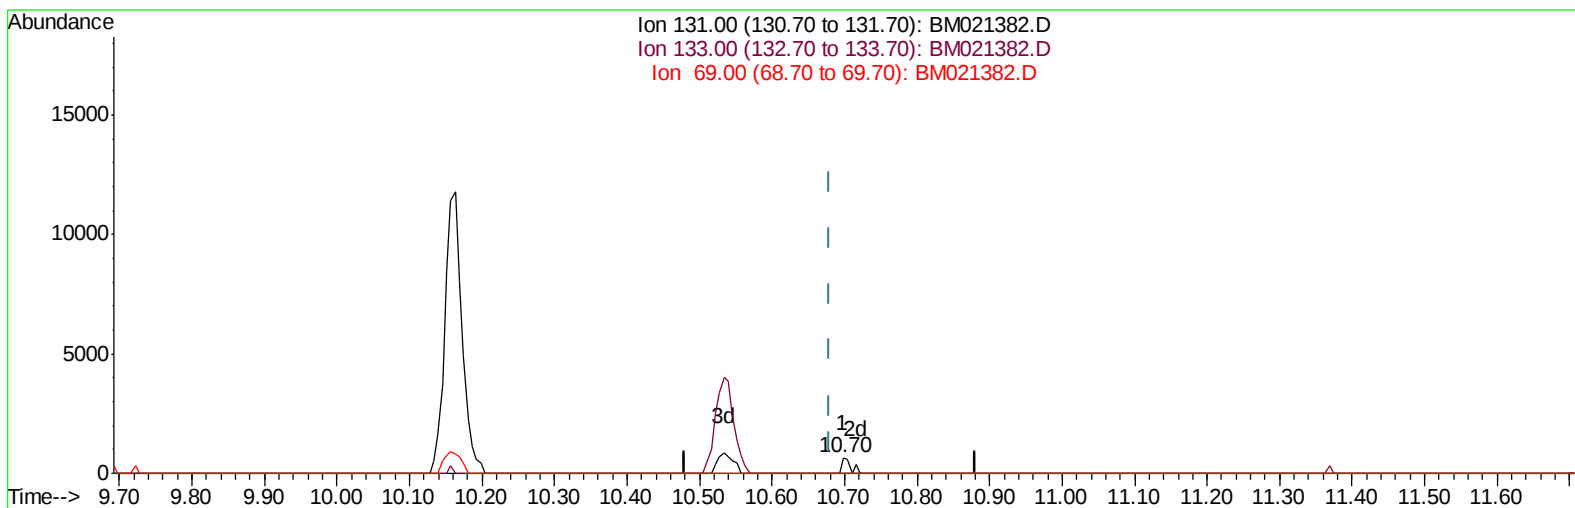




TIC: BM021382.D

(29) 4-Chloroaniline-d4 (S)
10.698min (+0.018) 0.02ng/ul
response 444

Ion	Exp%	Act%
131.00	100	100
133.00	33.20	0.00#
69.00	18.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021382.D
Acq On : 04 Jul 2019 01:05
Operator : HP/JU
Sample : K3462-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jul 04 01:56:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:58:18 2019
Response via : Initial Calibration

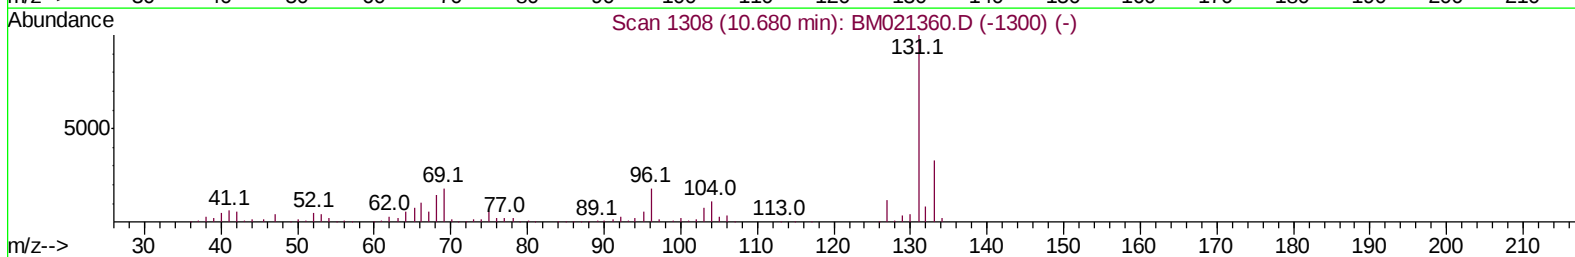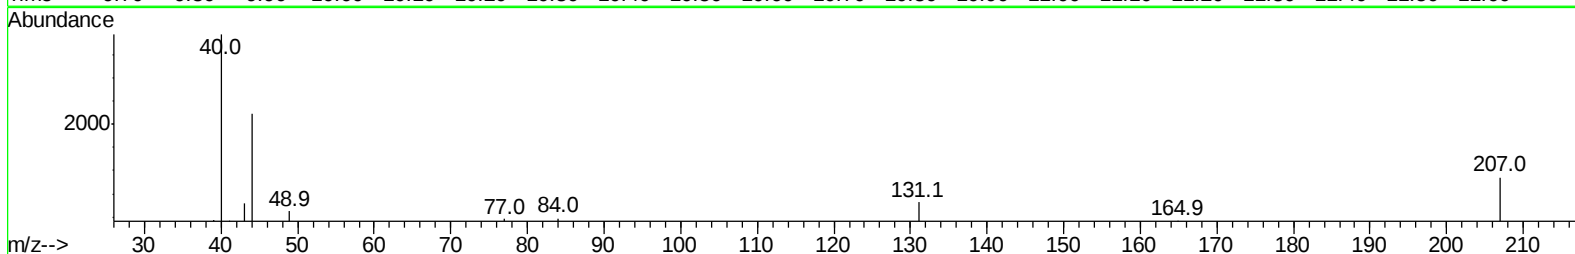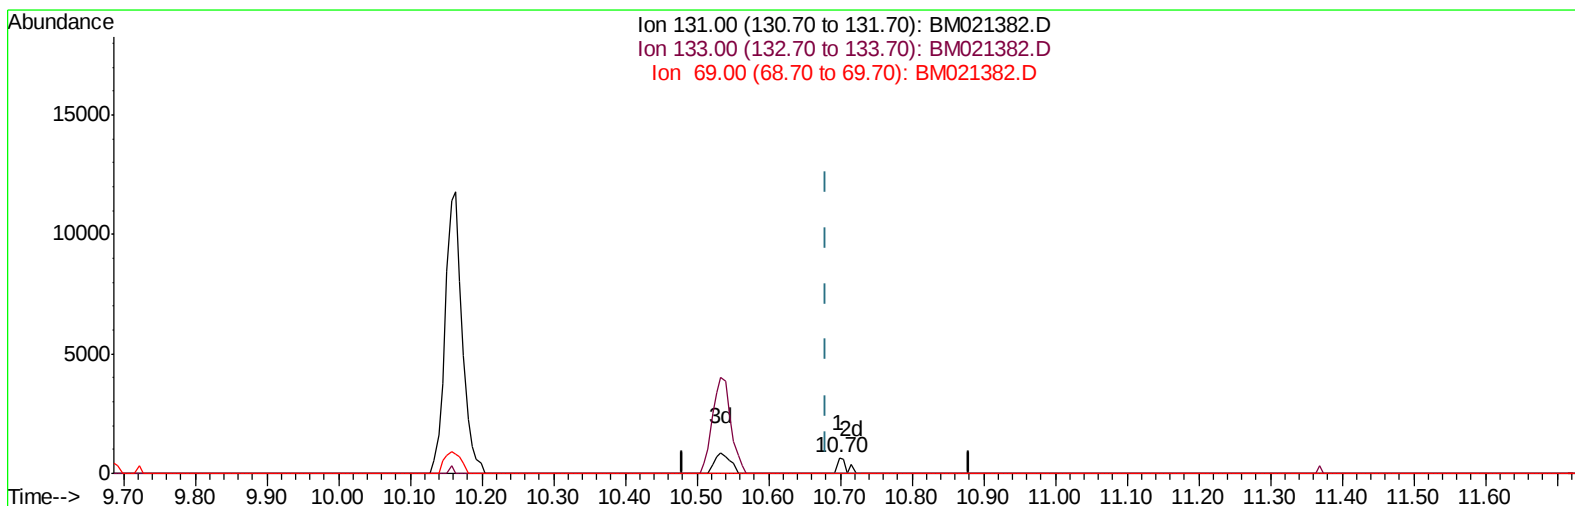

TIC: BM021382.D

(29) 4-Chloroaniline-d4 (S)

10.698min (+0.018) 0.03ng/ul m

response 573

Ion	Exp%	Act%
131.00	100	100
133.00	33.20	0.00#
69.00	18.00	0.00#
0.00	0.00	0.00