

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
 Data File : BM021362.D
 Acq On : 03 Jul 2019 10:28
 Operator : HP/JU
 Sample : K3497-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GAM07

Quant Time: Jul 03 15:33:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:58:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	201887	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	915933	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	560985	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1170866	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	942512	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1071769	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.28	96	10899	2.56	ng/uL	0.00
5) Phenol-d5	6.92	99	241293	13.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	144311	13.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	205655	14.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	180963	12.34	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	109051	14.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	127701	15.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	250491	14.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	212013	12.11	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	788041	15.55	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	891157	14.36	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	70601	8.56	ng/ul	0.00
57) Fluorene-d10	15.39	176	653867	14.83	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	64839	9.01	ng/ul	0.00
70) Anthracene-d10	17.24	188	890636	14.64	ng/ul	0.00
78) Pyrene-d10	19.53	212	899316	15.90	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.45	264	920111	14.55	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	13.85	163	259413	5.622	ng/ul	99
83) Bis(2-ethylhexyl)phthalate	21.23	149	78626	2.239	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021362.D
Acq On : 03 Jul 2019 10:28
Operator : HP/JU
Sample : K3497-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GAM07

Quant Time: Jul 03 15:33:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:58:18 2019
Response via : Initial Calibration

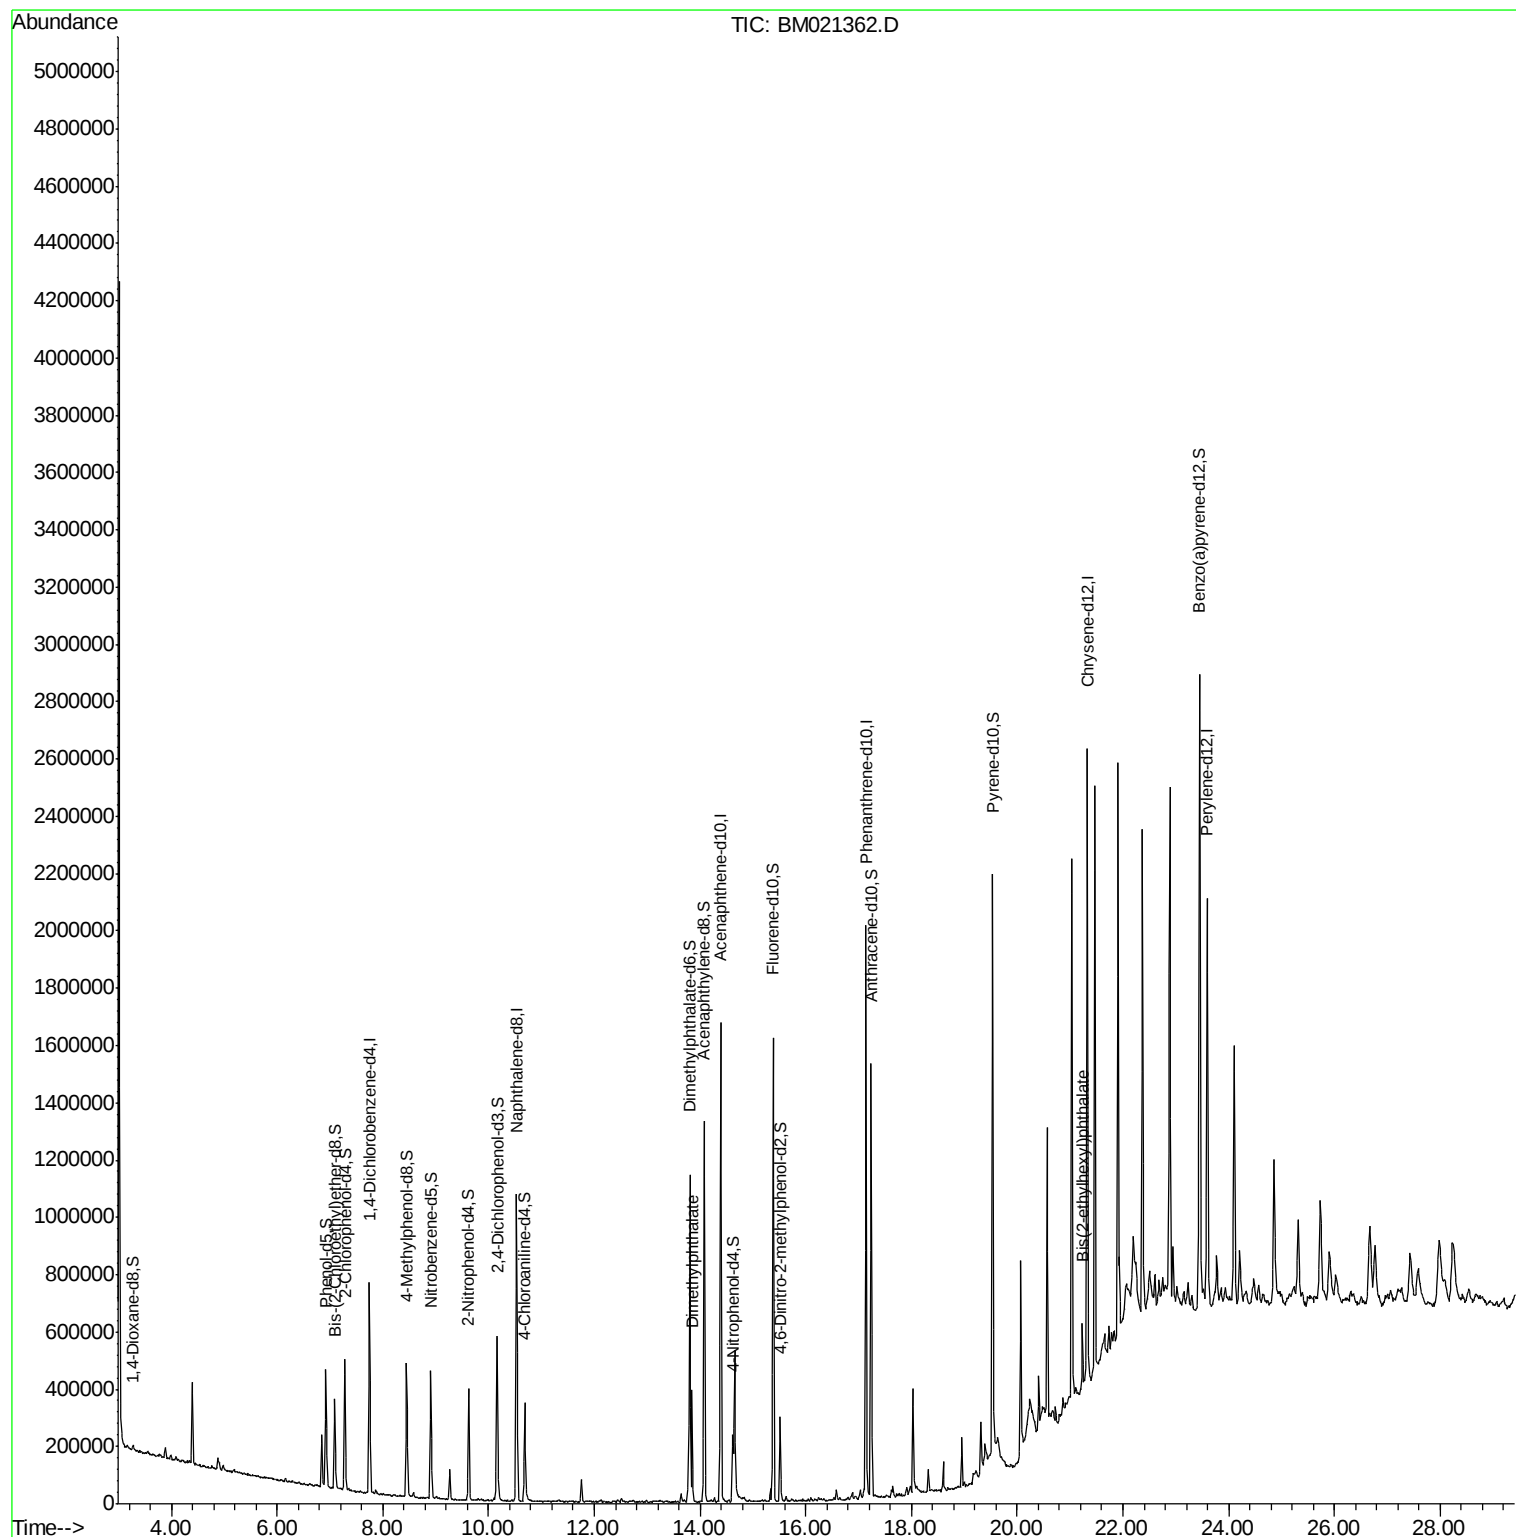

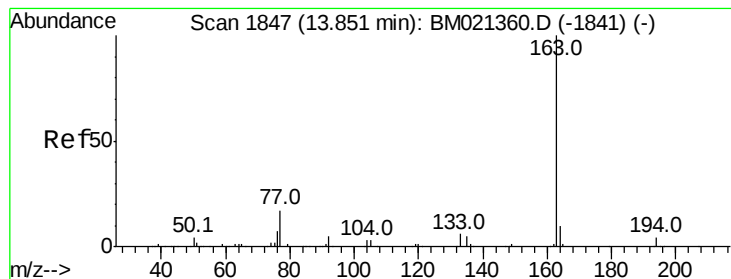

#44

Dimethylphthalate

Concen: 5.622 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. 0.00 min

Lab File: BM021362.D

Acq: 03 Jul 2019 10:28

Instrument :

BNA_M

ClientSampleId :

GAM07


Tot Ion:163 Resp: 259413

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2




164 10.1 7.7 11.5

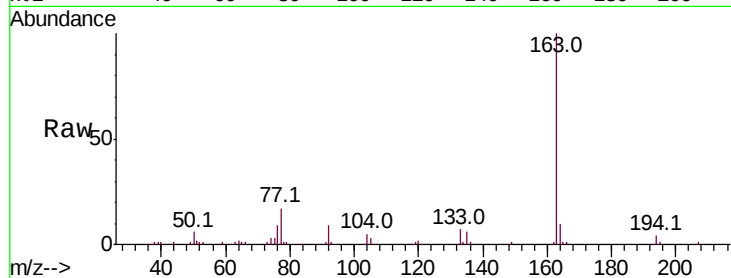

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

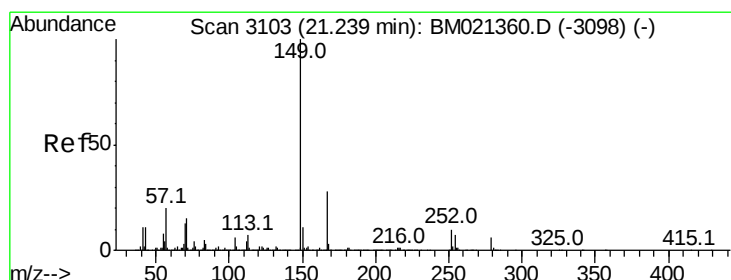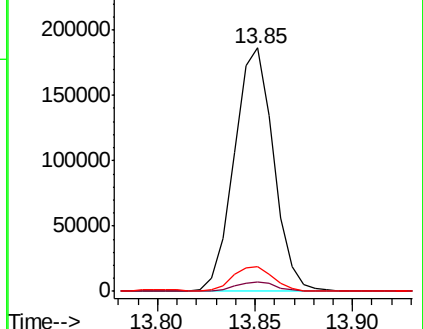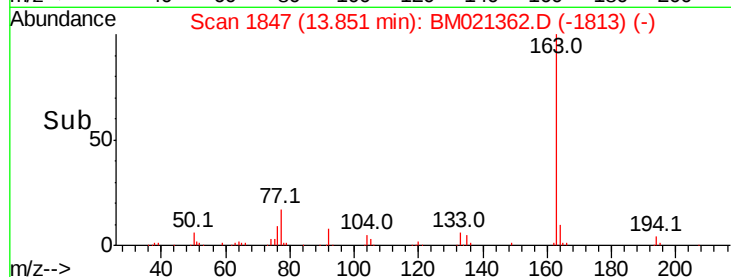

#83

Bis(2-ethylhexyl)phthalate

Concen: 2.239 ng/ul

RT: 21.23 min Scan# 3102

Delta R.T. 0.00 min

Lab File: BM021362.D

Acq: 03 Jul 2019 10:28


Tgt Ion:149 Resp: 78626

Ion Ratio Lower Upper

149 100

167 28.3 22.3 33.5

279 5.2 3.8 5.6

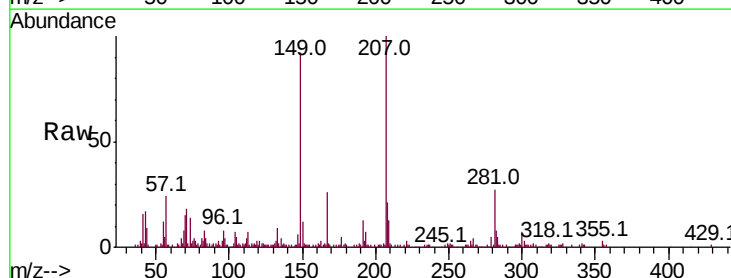

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

