

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
 Data File : BM021368.D
 Acq On : 03 Jul 2019 16:25
 Operator : HP/JU
 Sample : K3596-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJF1

Quant Time: Jul 03 17:17:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:58:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	204133	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	920824	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	565783	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1132805	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	954296	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1089624	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	18110	4.21	ng/uL	0.00
5) Phenol-d5	6.92	99	401593	22.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	234063	22.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	339791	23.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	357859	24.13	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	184768	24.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	216880	26.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	411319	24.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	510318	28.99	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	1286045	25.16	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	1481052	23.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	113415	13.64	ng/ul	0.00
57) Fluorene-d10	15.39	176	1053040	23.68	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	104312	14.98	ng/ul	0.00
70) Anthracene-d10	17.24	188	1438522	24.44	ng/ul	0.00
78) Pyrene-d10	19.53	212	1448475	25.29	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	1543053	24.00	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.85	163	380598	8.178	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021368.D
Acq On : 03 Jul 2019 16:25
Operator : HP/JU
Sample : K3596-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJF1

Quant Time: Jul 03 17:17:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:58:18 2019
Response via : Initial Calibration

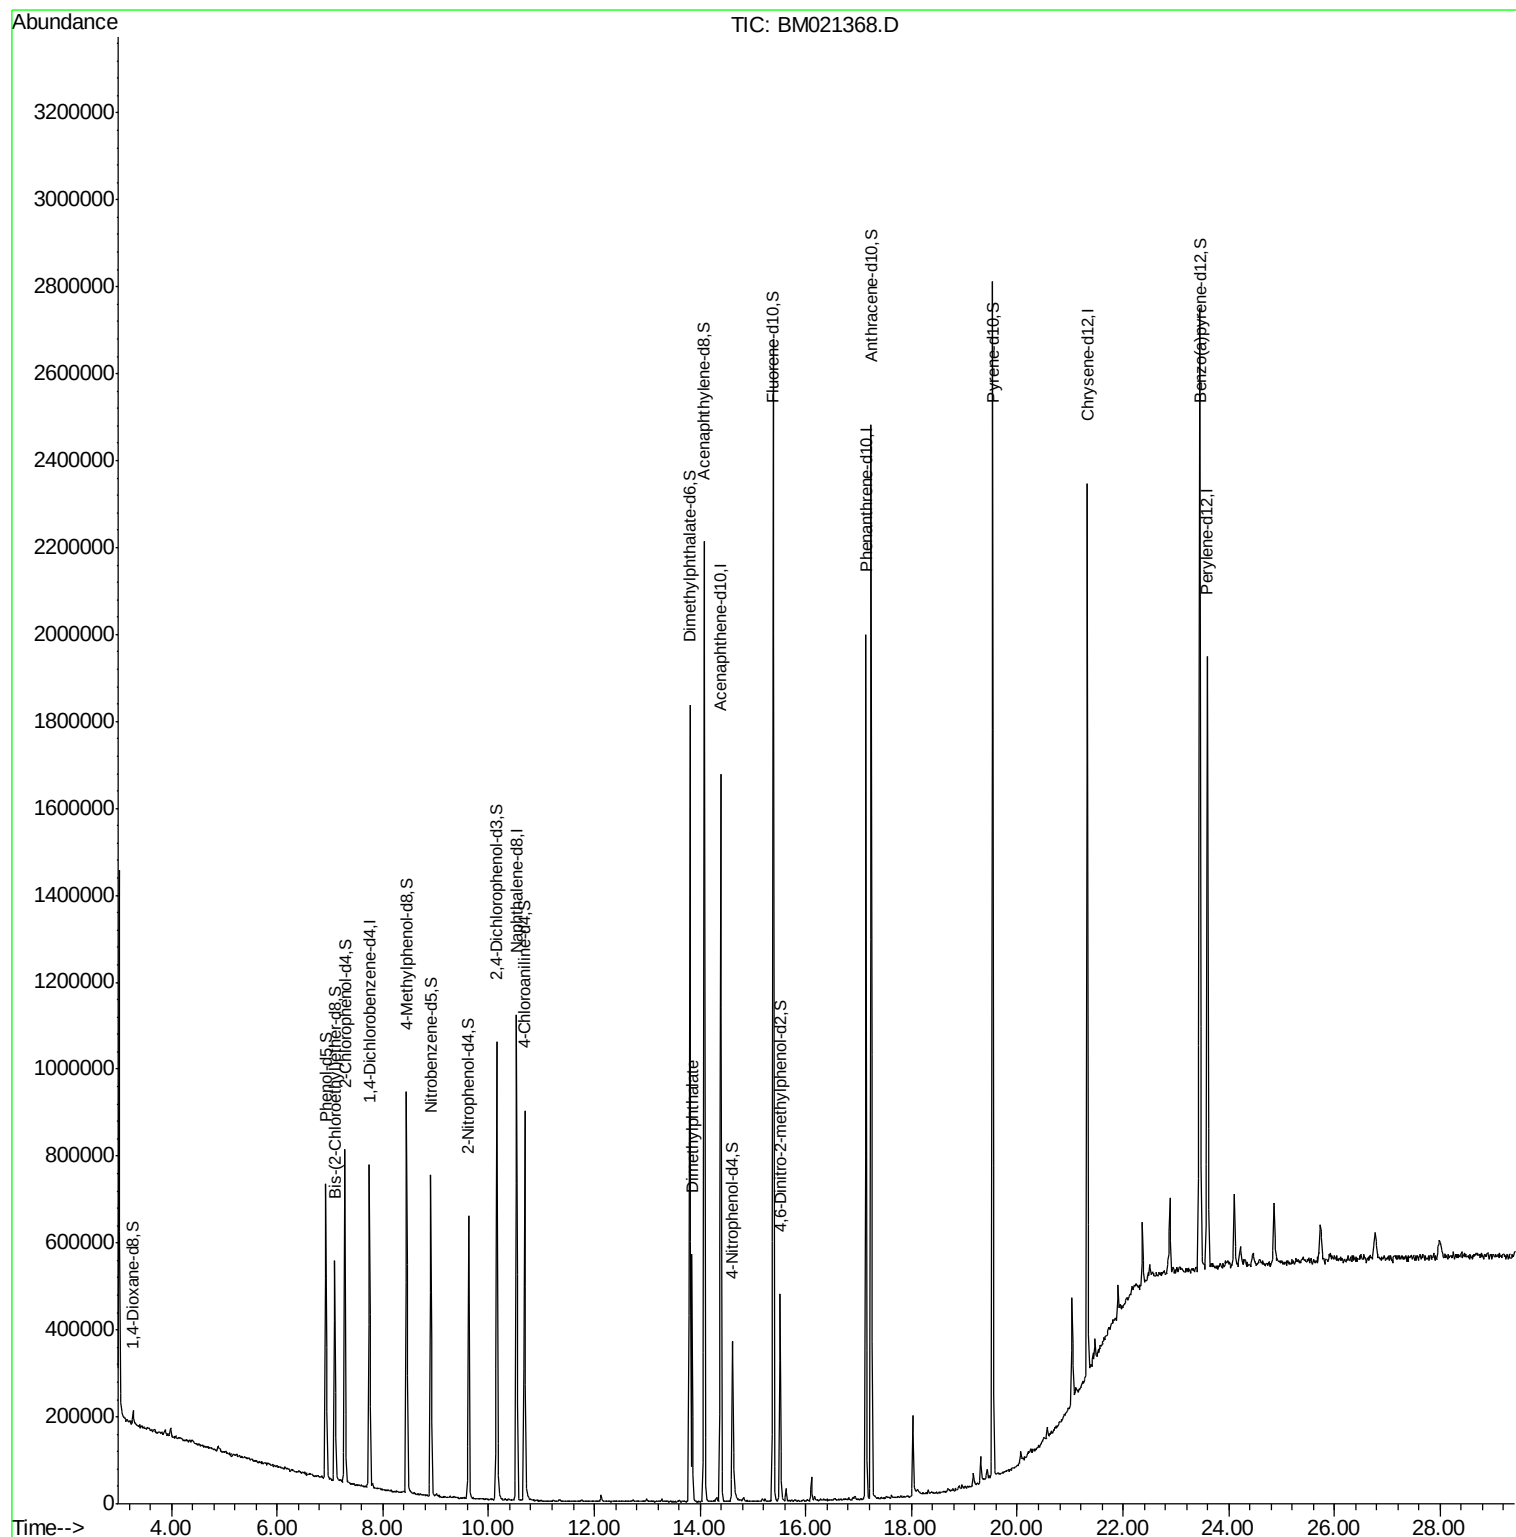

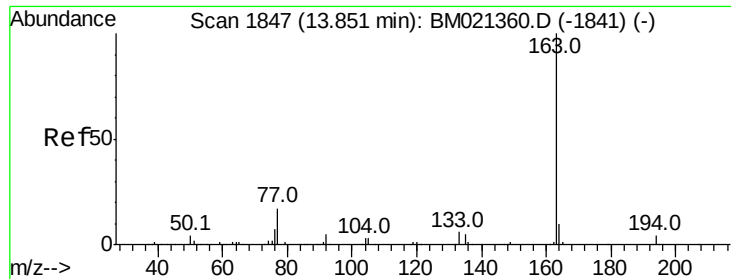

#44

Dimethylphthalate

Concen: 8.178 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. -0.00 min

Lab File: BM021368.D

Acq: 03 Jul 2019 16:25

Instrument :

BNA_M

ClientSampleId :

JLJF1


Tot Ion:163 Resp: 380598

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 10.0 7.7 11.5

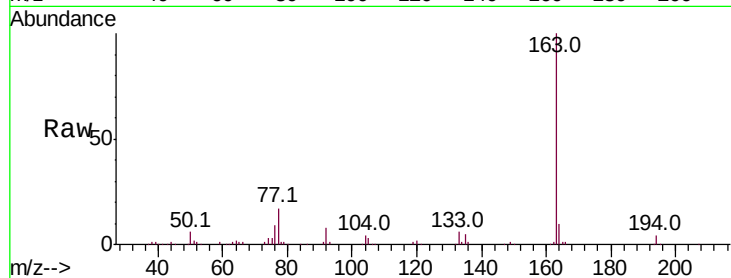

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

