

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
 Data File : BM021369.D
 Acq On : 03 Jul 2019 17:01
 Operator : HP/JU
 Sample : K3596-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJF3

Quant Time: Jul 03 17:47:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:58:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	181431	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	854894	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	559472	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1303553	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	996333	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1086310	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.28	96	17434	4.56	ng/uL	0.00
5) Phenol-d5	6.92	99	405667	25.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	231912	24.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	338704	26.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	359145	27.24	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	183176	26.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	216656	28.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	420505	26.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	521803	31.93	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	1338656	26.48	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	1573809	25.43	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	136992	16.66	ng/ul	0.00
57) Fluorene-d10	15.39	176	1183049	26.90	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	132182	16.50	ng/ul	0.00
70) Anthracene-d10	17.24	188	1760711	25.99	ng/ul	0.00
78) Pyrene-d10	19.53	212	1754850	29.35	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	1661810	25.93	ng/ul	0.00
Target Compounds						
6) Phenol	6.95	94	17303	1.158	ng/ul#	85
44) Dimethylphthalate	13.85	163	389351	8.461	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021369.D
Acq On : 03 Jul 2019 17:01
Operator : HP/JU
Sample : K3596-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJF3

Quant Time: Jul 03 17:47:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:58:18 2019
Response via : Initial Calibration

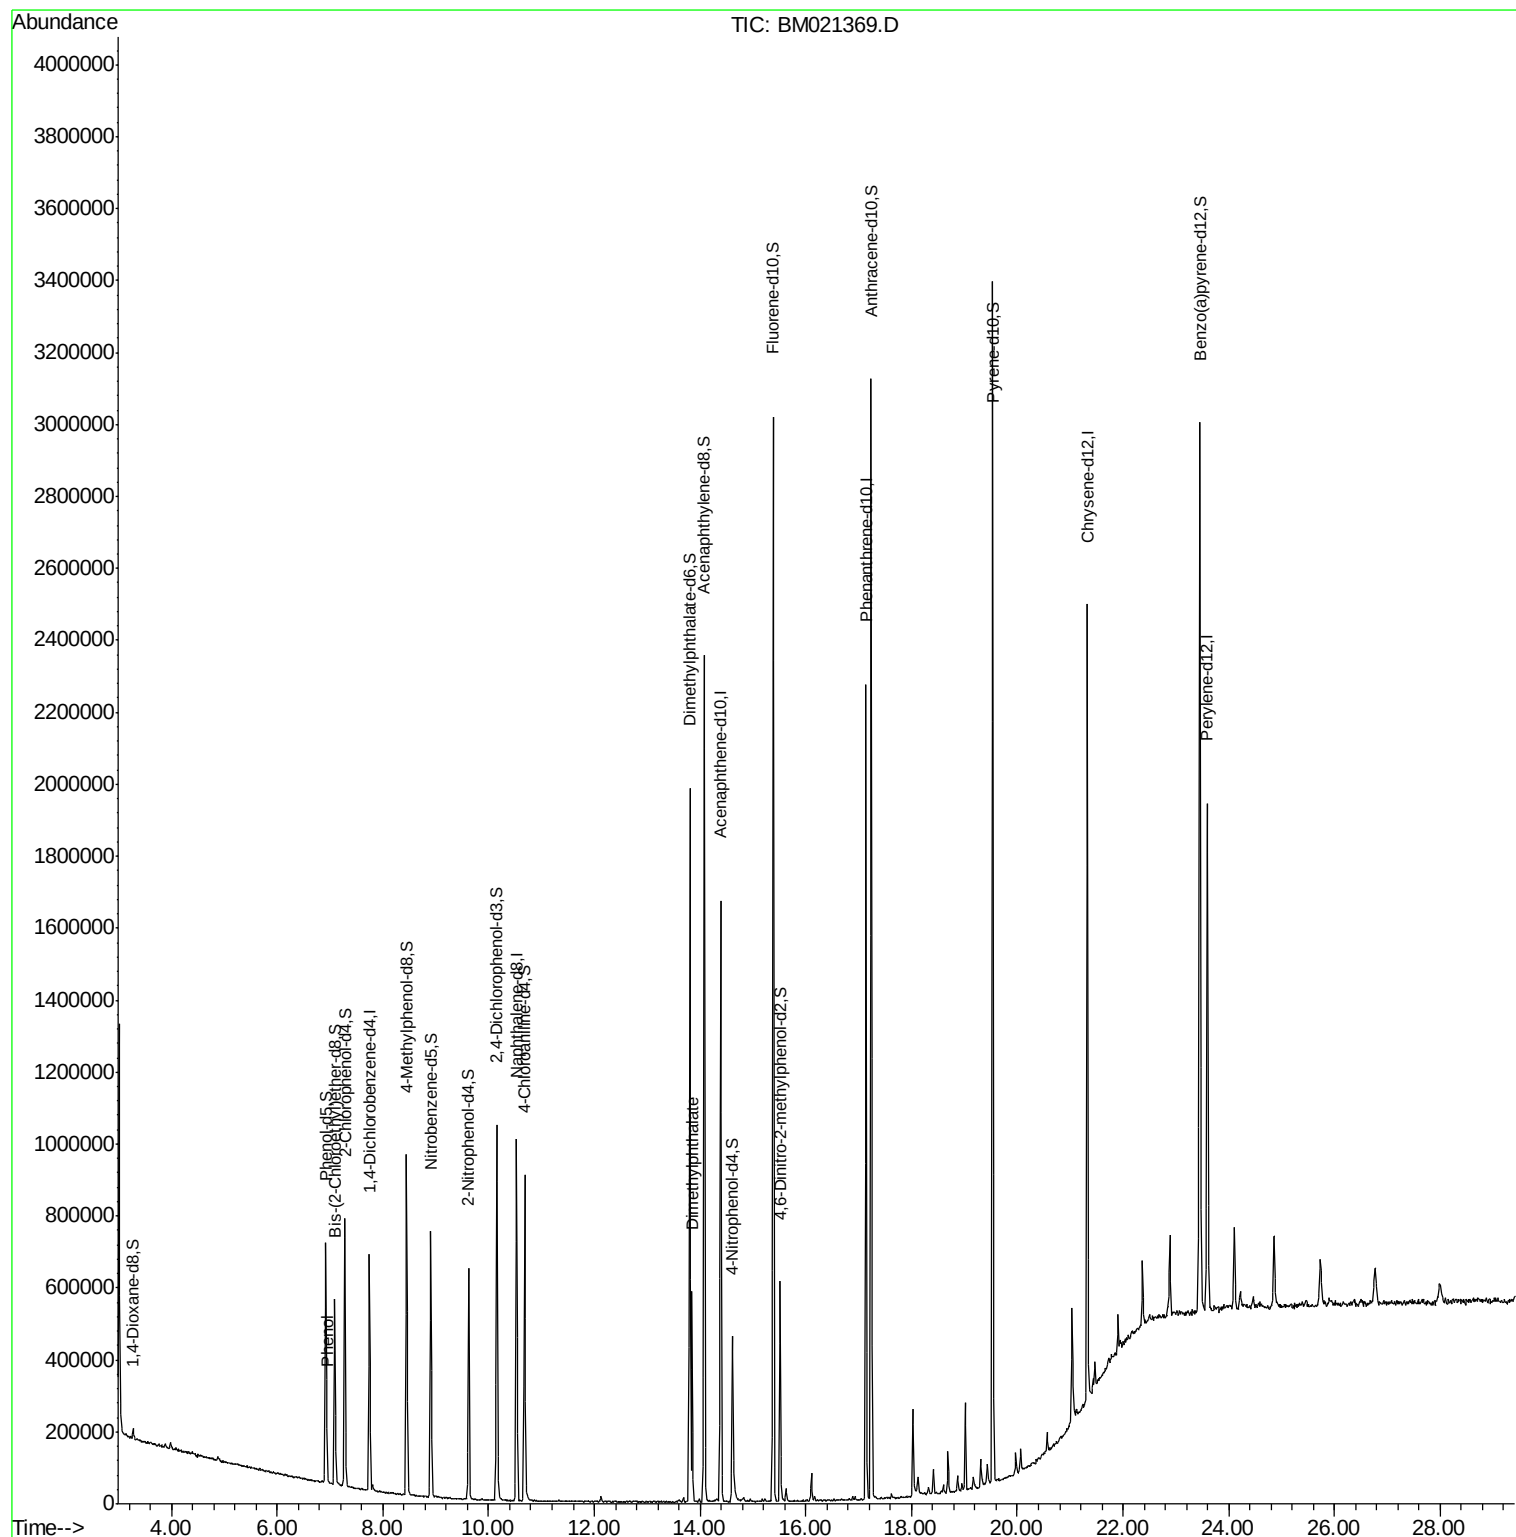

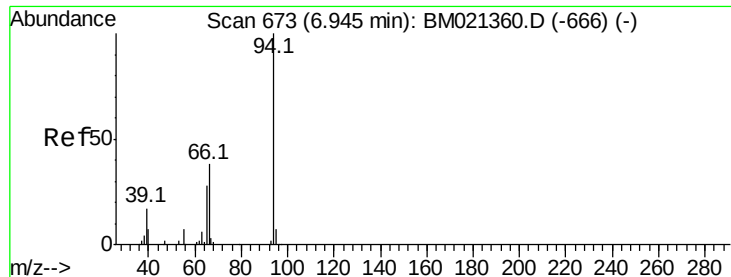

#6

Phenol

Concen: 1.158 ng/ul

RT: 6.95 min Scan# 673

Delta R.T. 0.00 min

Lab File: BM021369.D

Acq: 03 Jul 2019 17:01

Instrument :

BNA_M

ClientSampleId :

JLJF3





Tot Ion: 94 Resp: 17303

Ion Ratio Lower Upper

94 100

65 33.2 22.6 34.0

66 50.7 31.2 46.8#

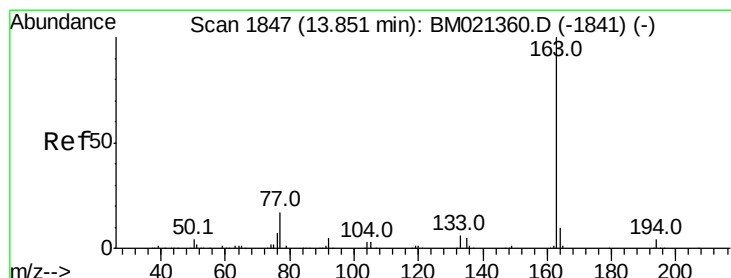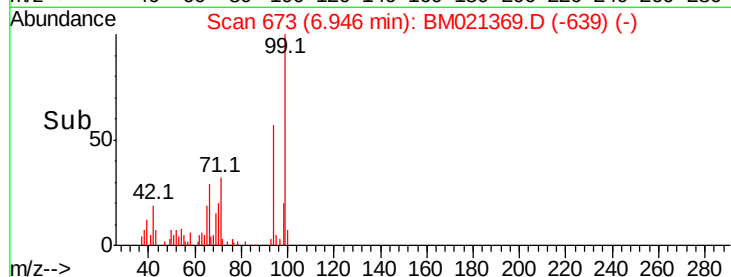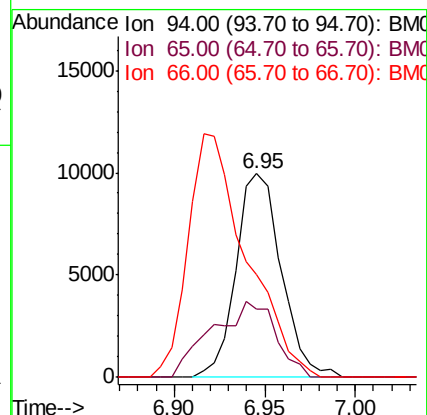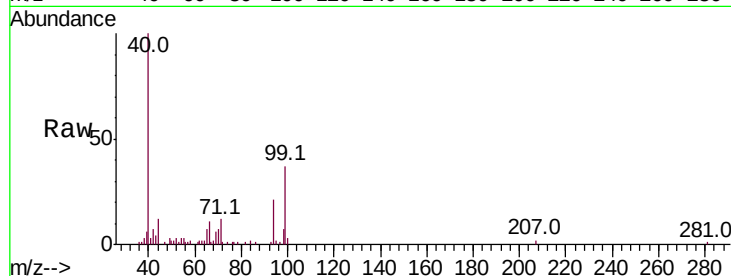

#44

Dimethylphthalate

Concen: 8.461 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. 0.00 min

Lab File: BM021369.D

Acq: 03 Jul 2019 17:01

Tgt Ion:163 Resp: 389351

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 9.5 7.7 11.5

