

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
 Data File : BM021371.D
 Acq On : 03 Jul 2019 18:14
 Operator : HP/JU
 Sample : K3596-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJF5

Quant Time: Jul 03 23:34:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:58:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	209491	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	939812	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	585200	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1131136	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	893060	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1064793	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	22187	5.03	ng/uL	0.00
5) Phenol-d5	6.92	99	490999	26.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	287097	26.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	419309	28.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	440343	28.93	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	225528	29.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	264695	31.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	502765	29.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	621608	34.60	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	1530989	28.95	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	1786141	27.59	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	131279	15.26	ng/ul	0.00
57) Fluorene-d10	15.39	176	1268761	27.59	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	123232	17.72	ng/ul	0.00
70) Anthracene-d10	17.24	188	1657225	28.19	ng/ul	0.00
78) Pyrene-d10	19.54	212	1584891	29.57	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.45	264	1789616	28.49	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.95	94	20782	1.205	ng/ul# 86
44) Dimethylphthalate	13.85	163	550141	11.429	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021371.D
Acq On : 03 Jul 2019 18:14
Operator : HP/JU
Sample : K3596-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJF5

Quant Time: Jul 03 23:34:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:58:18 2019
Response via : Initial Calibration

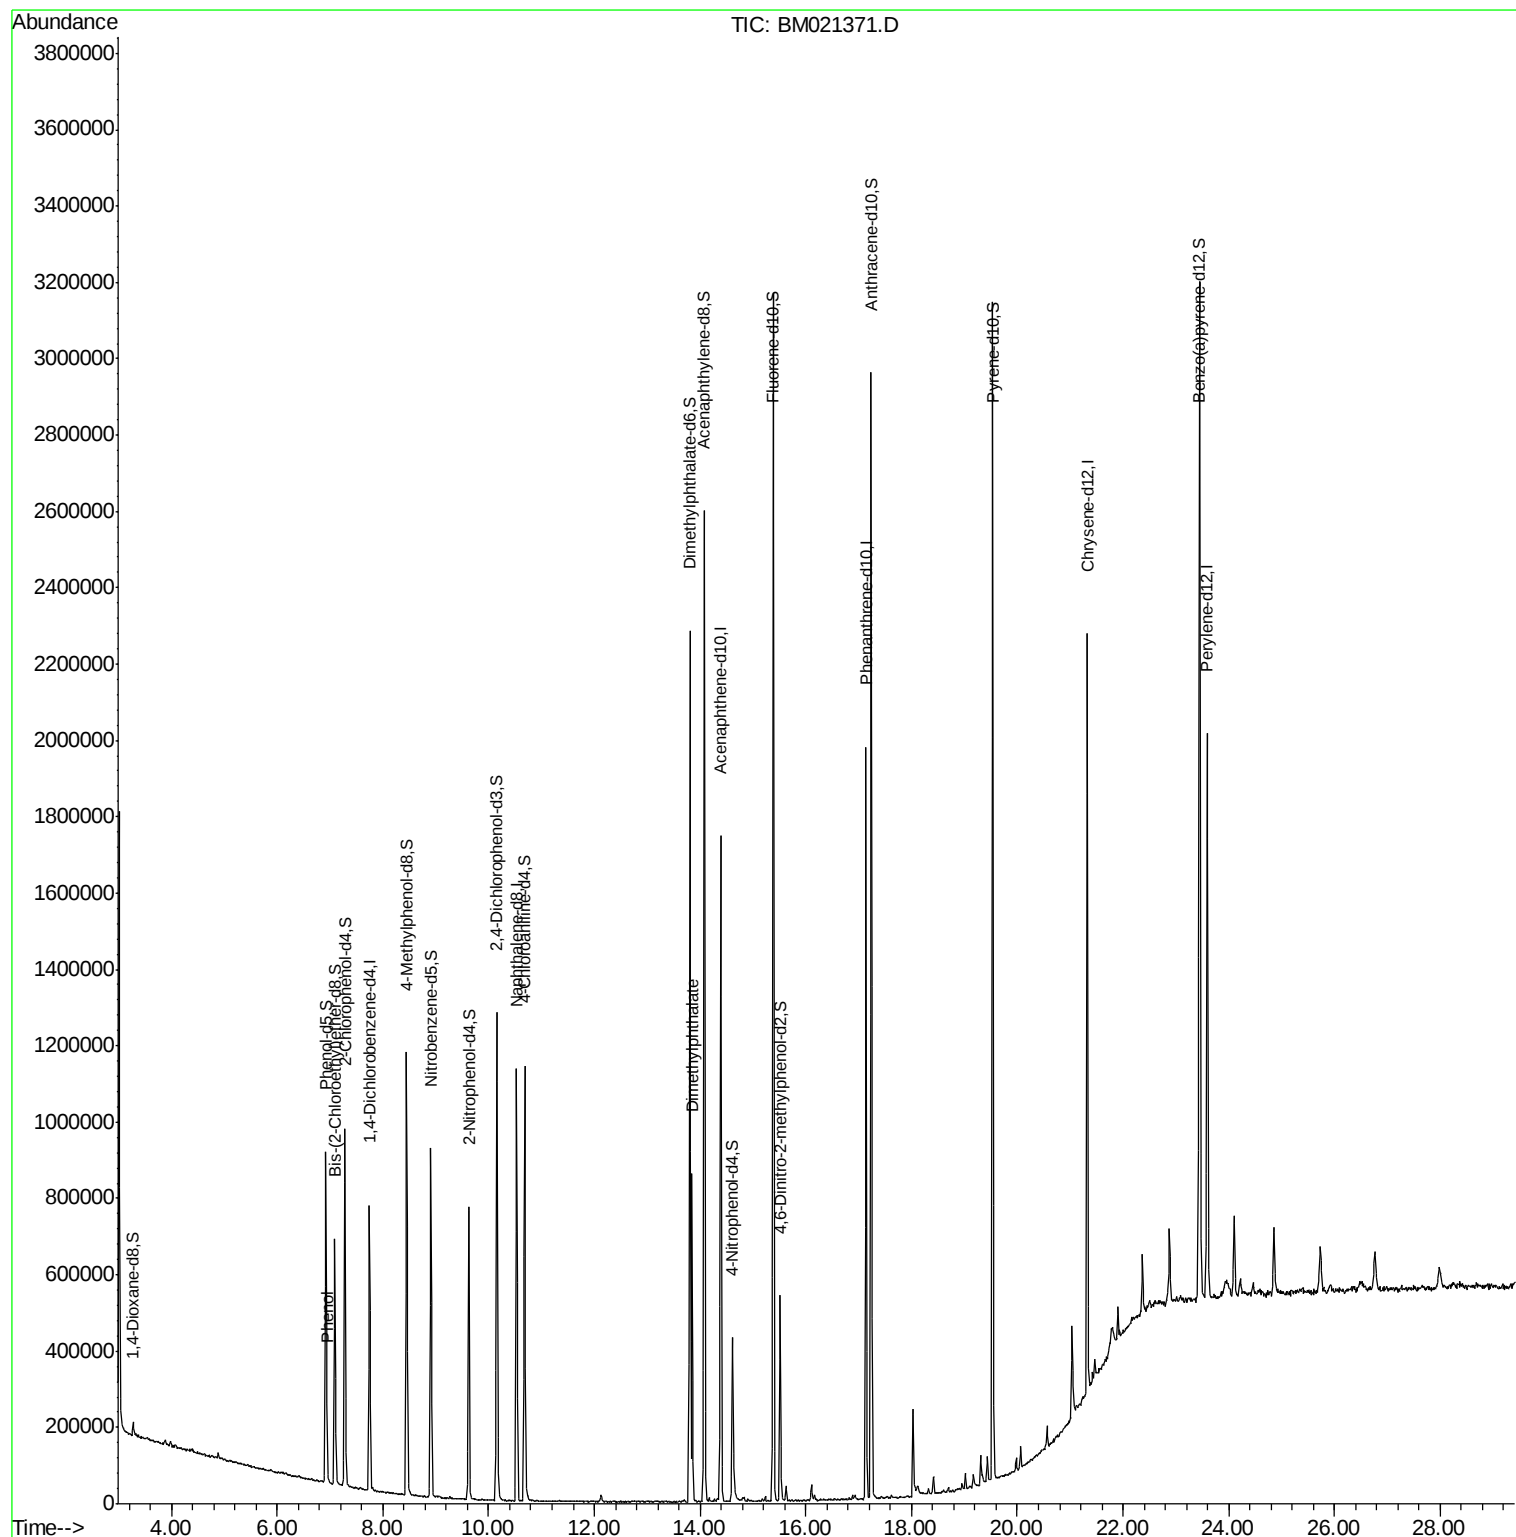

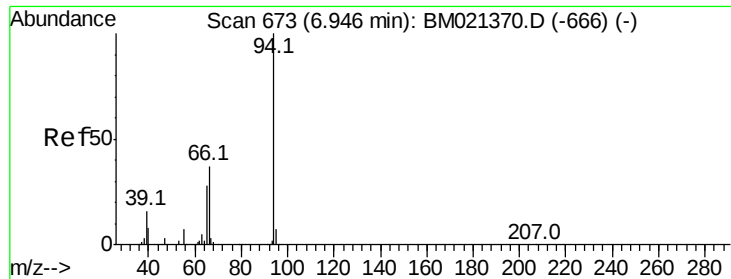

#6

Phenol

Concen: 1.205 ng/ul

RT: 6.95 min Scan# 673

Delta R.T. -0.00 min

Lab File: BM021371.D

Acq: 03 Jul 2019 18:14

Instrument :

BNA_M

ClientSampleId :

JLJF5





Tot Ion: 94 Resp: 20782

Ion Ratio Lower Upper

94 100

65 32.1 22.6 34.0

66 50.4 31.2 46.8#

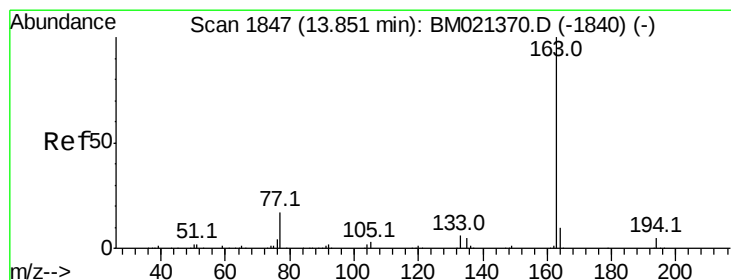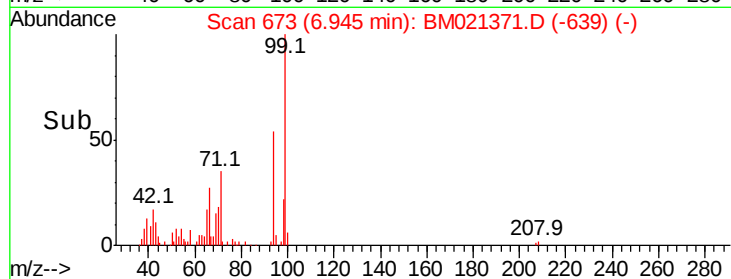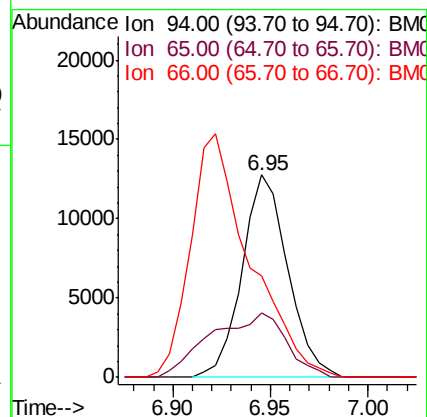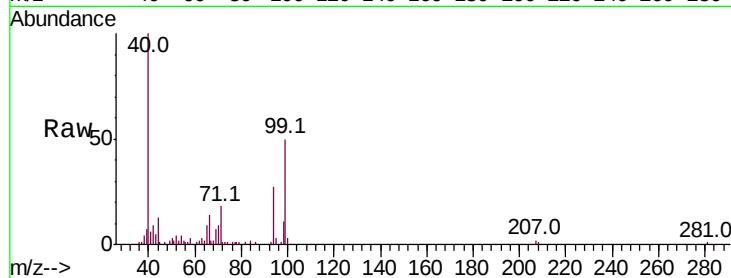

#44

Dimethylphthalate

Concen: 11.429 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. -0.00 min

Lab File: BM021371.D

Acq: 03 Jul 2019 18:14

Tgt Ion:163 Resp: 550141

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 9.9 7.7 11.5

