

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
 Data File : BM021374.D
 Acq On : 03 Jul 2019 20:06
 Operator : HP/JU
 Sample : K3596-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJG0

Quant Time: Jul 03 23:34:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:58:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	229261	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	1010807	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	616006	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1190267	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	964923	20.00	ng/ul	0.00
85) Perylene-d12	23.59	264	1138473	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	21660	4.49	ng/uL	0.00
5) Phenol-d5	6.92	99	464244	23.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	268753	22.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	398611	24.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	408492	24.52	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	208256	25.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	240916	26.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	458488	24.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	569824	29.49	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	1382352	24.84	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	1616340	23.72	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	119300	13.18	ng/ul	0.00
57) Fluorene-d10	15.39	176	1151584	23.79	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	104149	14.23	ng/ul	0.00
70) Anthracene-d10	17.24	188	1493569	24.15	ng/ul	0.00
78) Pyrene-d10	19.53	212	1452070	25.08	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.45	264	1631272	24.29	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.85	163	405954	8.012	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021374.D
Acq On : 03 Jul 2019 20:06
Operator : HP/JU
Sample : K3596-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJG0

Quant Time: Jul 03 23:34:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:58:18 2019
Response via : Initial Calibration

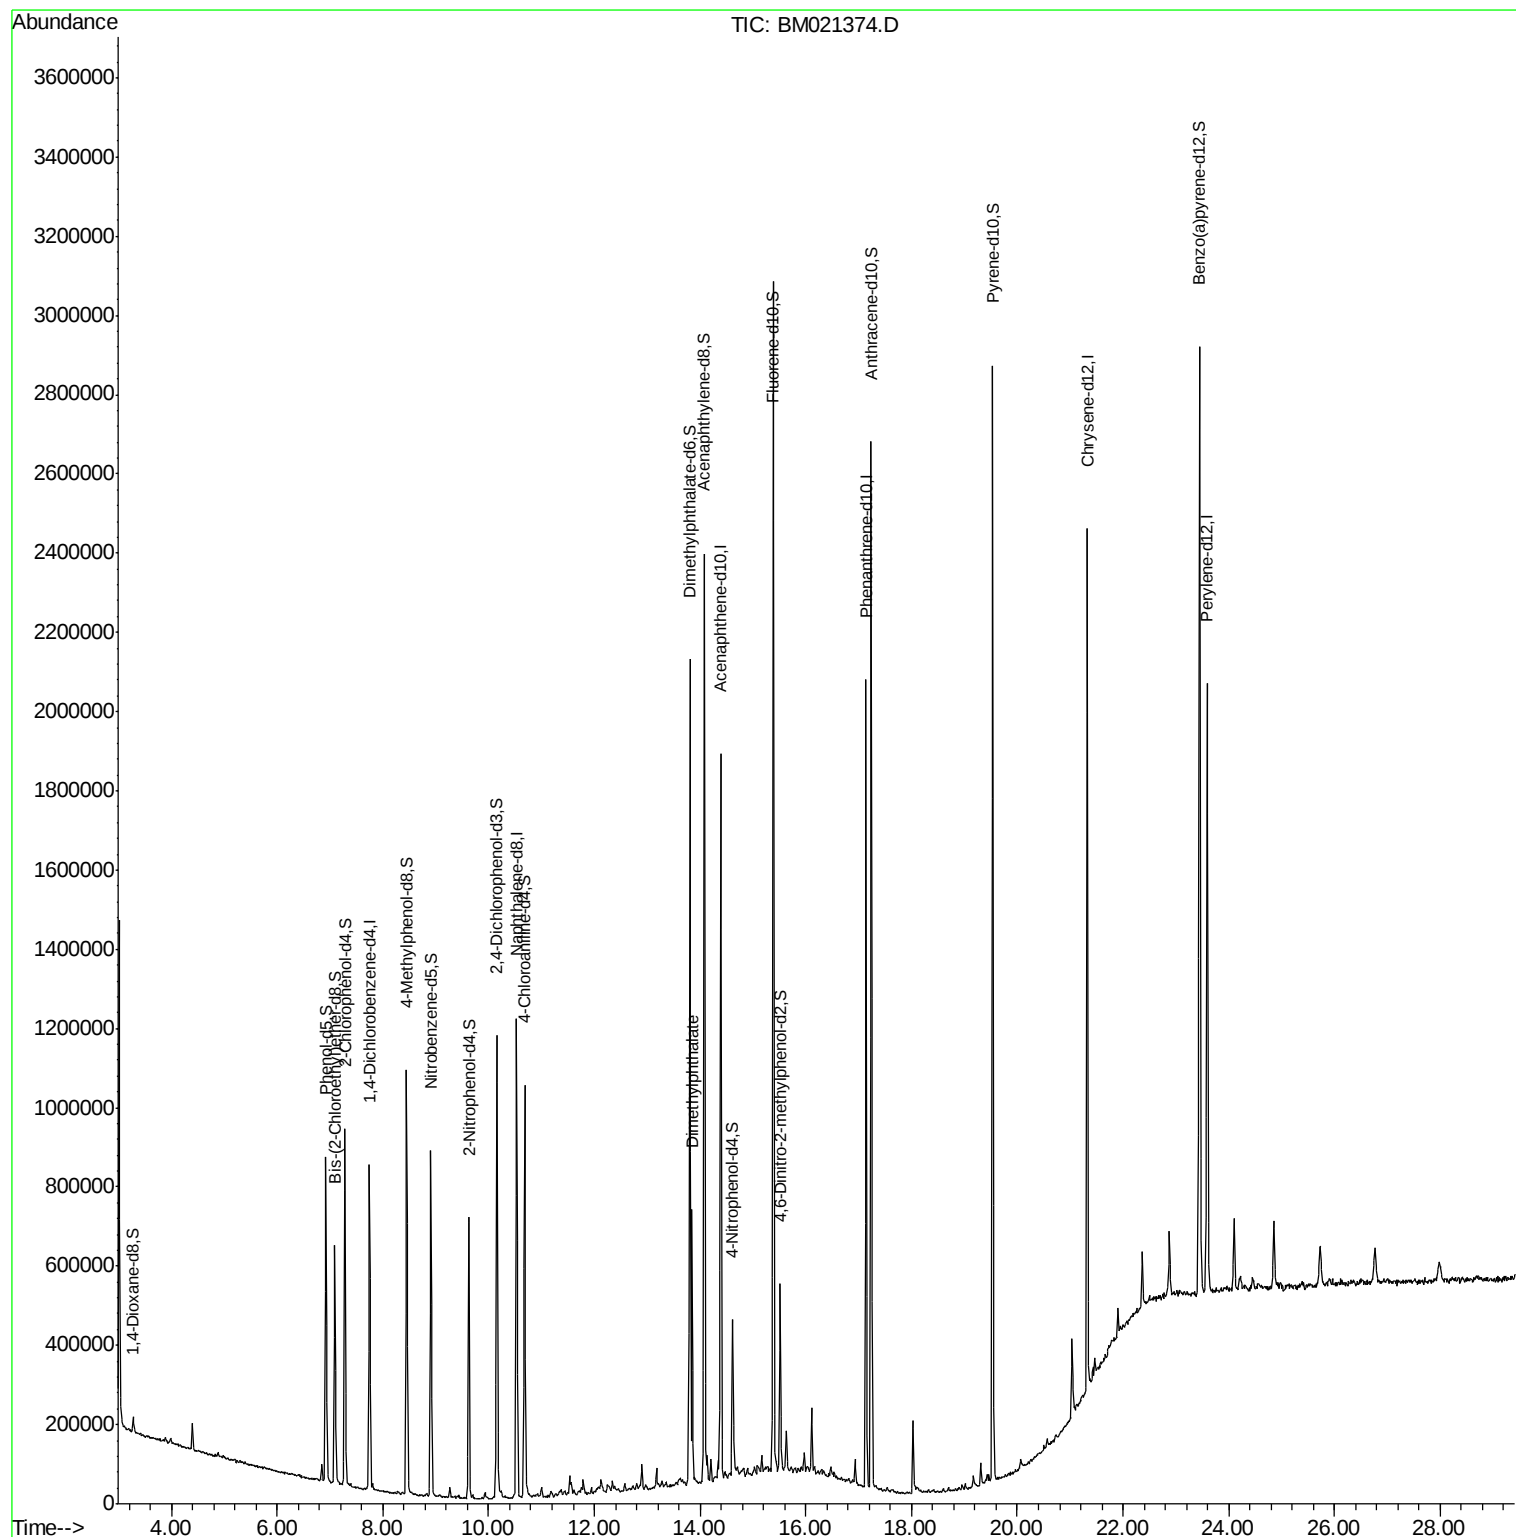

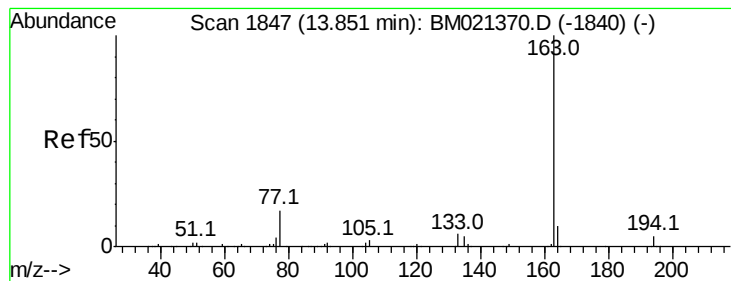

#44

Dimethylphthalate

Concen: 8.012 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. 0.00 min

Lab File: BM021374.D

Acq: 03 Jul 2019 20:06

Instrument :

BNA_M

ClientSampleId :

JLJG0


Tot Ion:163 Resp: 405954

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2

164 10.0 7.7 11.5

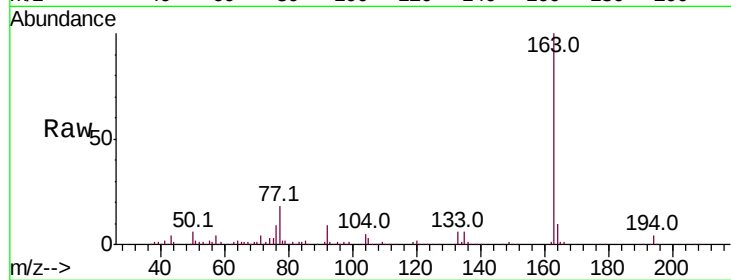

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

