

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
 Data File : BM021377.D
 Acq On : 03 Jul 2019 21:58
 Operator : HP/JU
 Sample : K3596-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLJG4

Quant Time: Jul 03 23:34:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:58:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	206098	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	924806	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	554333	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1046659	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	853123	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1017044	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	22435	5.17	ng/uL	0.00
5) Phenol-d5	6.92	99	136976	7.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	301246	28.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	372521	25.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	261951	17.49	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	238760	31.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	273357	32.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	504549	29.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	68138	3.85	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	1682665	33.59	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	1949083	31.79	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	32576	4.00	ng/ul	0.01
57) Fluorene-d10	15.39	176	1397766	32.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	153793	23.90	ng/ul	0.00
70) Anthracene-d10	17.24	188	1942457	35.71	ng/ul	0.00
78) Pyrene-d10	19.54	212	1869439	36.52	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.45	264	2172919	36.21	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.85	163	83922	1.841	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021377.D
Acq On : 03 Jul 2019 21:58
Operator : HP/JU
Sample : K3596-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLJG4

Quant Time: Jul 03 23:34:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:58:18 2019
Response via : Initial Calibration

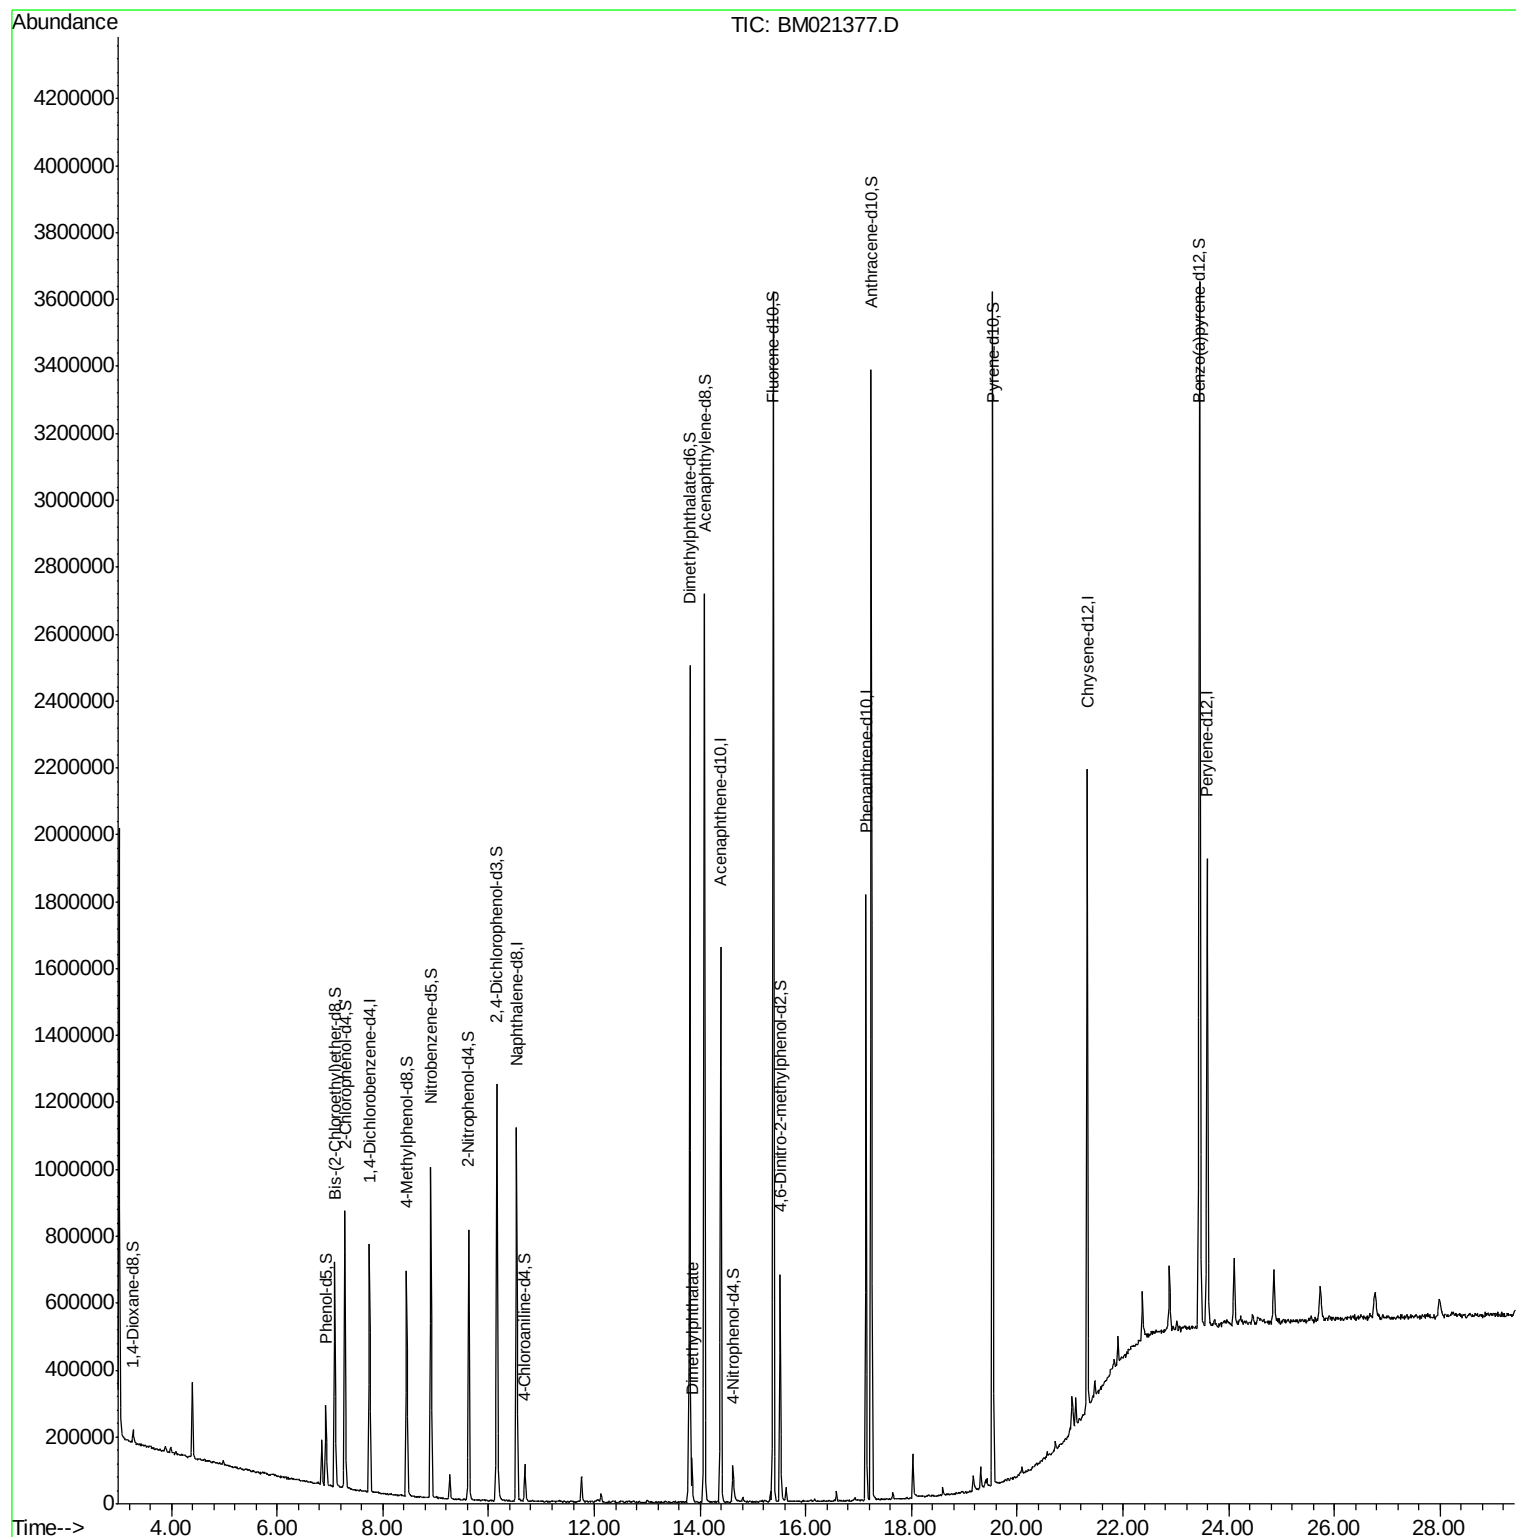

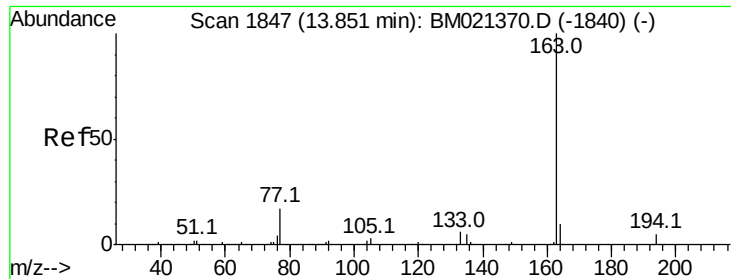

#44

Dimethylphthalate

Concen: 1.841 ng/ul

RT: 13.85 min Scan# 1847

Delta R.T. 0.00 min

Lab File: BM021377.D

Acq: 03 Jul 2019 21:58

Instrument :

BNA_M

ClientSampleId :

JLJG4


Tot Ion:163 Resp: 83922

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2

164 10.1 7.7 11.5

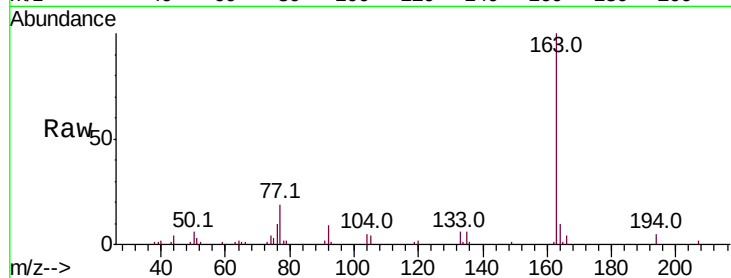

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

