

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
 Data File : BM021366.D
 Acq On : 03 Jul 2019 15:12
 Operator : HP/JU
 Sample : PB121053BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK53

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.922	663	669	683	rVB	890017	1414291	28.24%	2.506%
2	7.093	692	698	708	rVB	667636	1060842	21.18%	1.880%
3	7.281	724	730	742	rVB	946663	1488739	29.73%	2.638%
4	7.746	803	809	817	rVB	688194	1109647	22.16%	1.966%
5	8.457	923	930	942	rBV	1155236	1944720	38.84%	3.446%
6	8.910	1000	1007	1020	rVB	953721	1560830	31.17%	2.766%
7	9.628	1122	1129	1143	rVB	829746	1364567	27.25%	2.418%
8	10.157	1212	1219	1237	rBV	1296427	2227472	44.48%	3.947%
9	10.534	1275	1283	1291	rBV	1102340	1796227	35.87%	3.183%
10	10.681	1301	1308	1325	rBV	1187918	2132586	42.59%	3.779%
11	12.128	1548	1554	1561	rVB2	19705	33775	0.67%	0.060%
12	12.381	1593	1597	1602	rBV3	5443	8530	0.17%	0.015%
13	13.357	1759	1763	1767	rBV2	3857	5459	0.11%	0.010%
14	13.804	1832	1839	1851	rBV	2376695	3303153	65.96%	5.853%
15	14.086	1879	1887	1897	rBV	2757834	4116124	82.20%	7.293%
16	14.392	1932	1939	1948	rBV2	1736869	2618921	52.30%	4.640%
17	14.610	1969	1976	1999	rBV	543744	1082201	21.61%	1.918%
18	14.763	1999	2002	2006	rVB3	4772	6919	0.14%	0.012%
19	15.386	2101	2108	2119	rBV	3417159	4900177	97.86%	8.683%
20	15.522	2125	2131	2144	rBV	689104	963494	19.24%	1.707%
21	15.628	2144	2149	2155	rVB	35219	52768	1.05%	0.093%
22	16.175	2237	2242	2245	rBV	12065	13928	0.28%	0.025%
23	16.927	2365	2370	2375	rBV4	7474	12381	0.25%	0.022%
24	17.027	2383	2387	2390	rBV5	3538	5430	0.11%	0.010%
25	17.145	2400	2407	2413	rBV	1984938	2835713	56.63%	5.025%
26	17.239	2417	2423	2436	rVV	3309760	4578904	91.44%	8.113%
27	18.027	2554	2557	2560	rBV4	5205	5445	0.11%	0.010%
28	18.380	2613	2617	2624	rBV2	11448	21838	0.44%	0.039%
29	19.174	2747	2752	2756	rBV	29983	47555	0.95%	0.084%
30	19.427	2791	2795	2798	rBV2	25758	34267	0.68%	0.061%
31	19.539	2808	2814	2822	rBV	3746258	4973071	99.31%	8.812%
32	21.115	3078	3082	3087	rBV	103934	146913	2.93%	0.260%
33	21.333	3114	3119	3125	rBV	2092236	2721752	54.35%	4.823%
34	23.456	3473	3480	3488	rBV	2778071	5007550	100.00%	8.873%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021366.D
Acq On : 03 Jul 2019 15:12
Operator : HP/JU
Sample : PB121053BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK53

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Title : SVOA CALIBRATION

35	23.604	3498	3505	3513	rVB	1526547	2840373	56.72%	5.033%
----	--------	------	------	------	-----	---------	---------	--------	--------


Sum of corrected areas: 56436562

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021366.D
Acq On : 03 Jul 2019 15:12
Operator : HP/JU
Sample : PB121053BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK53

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

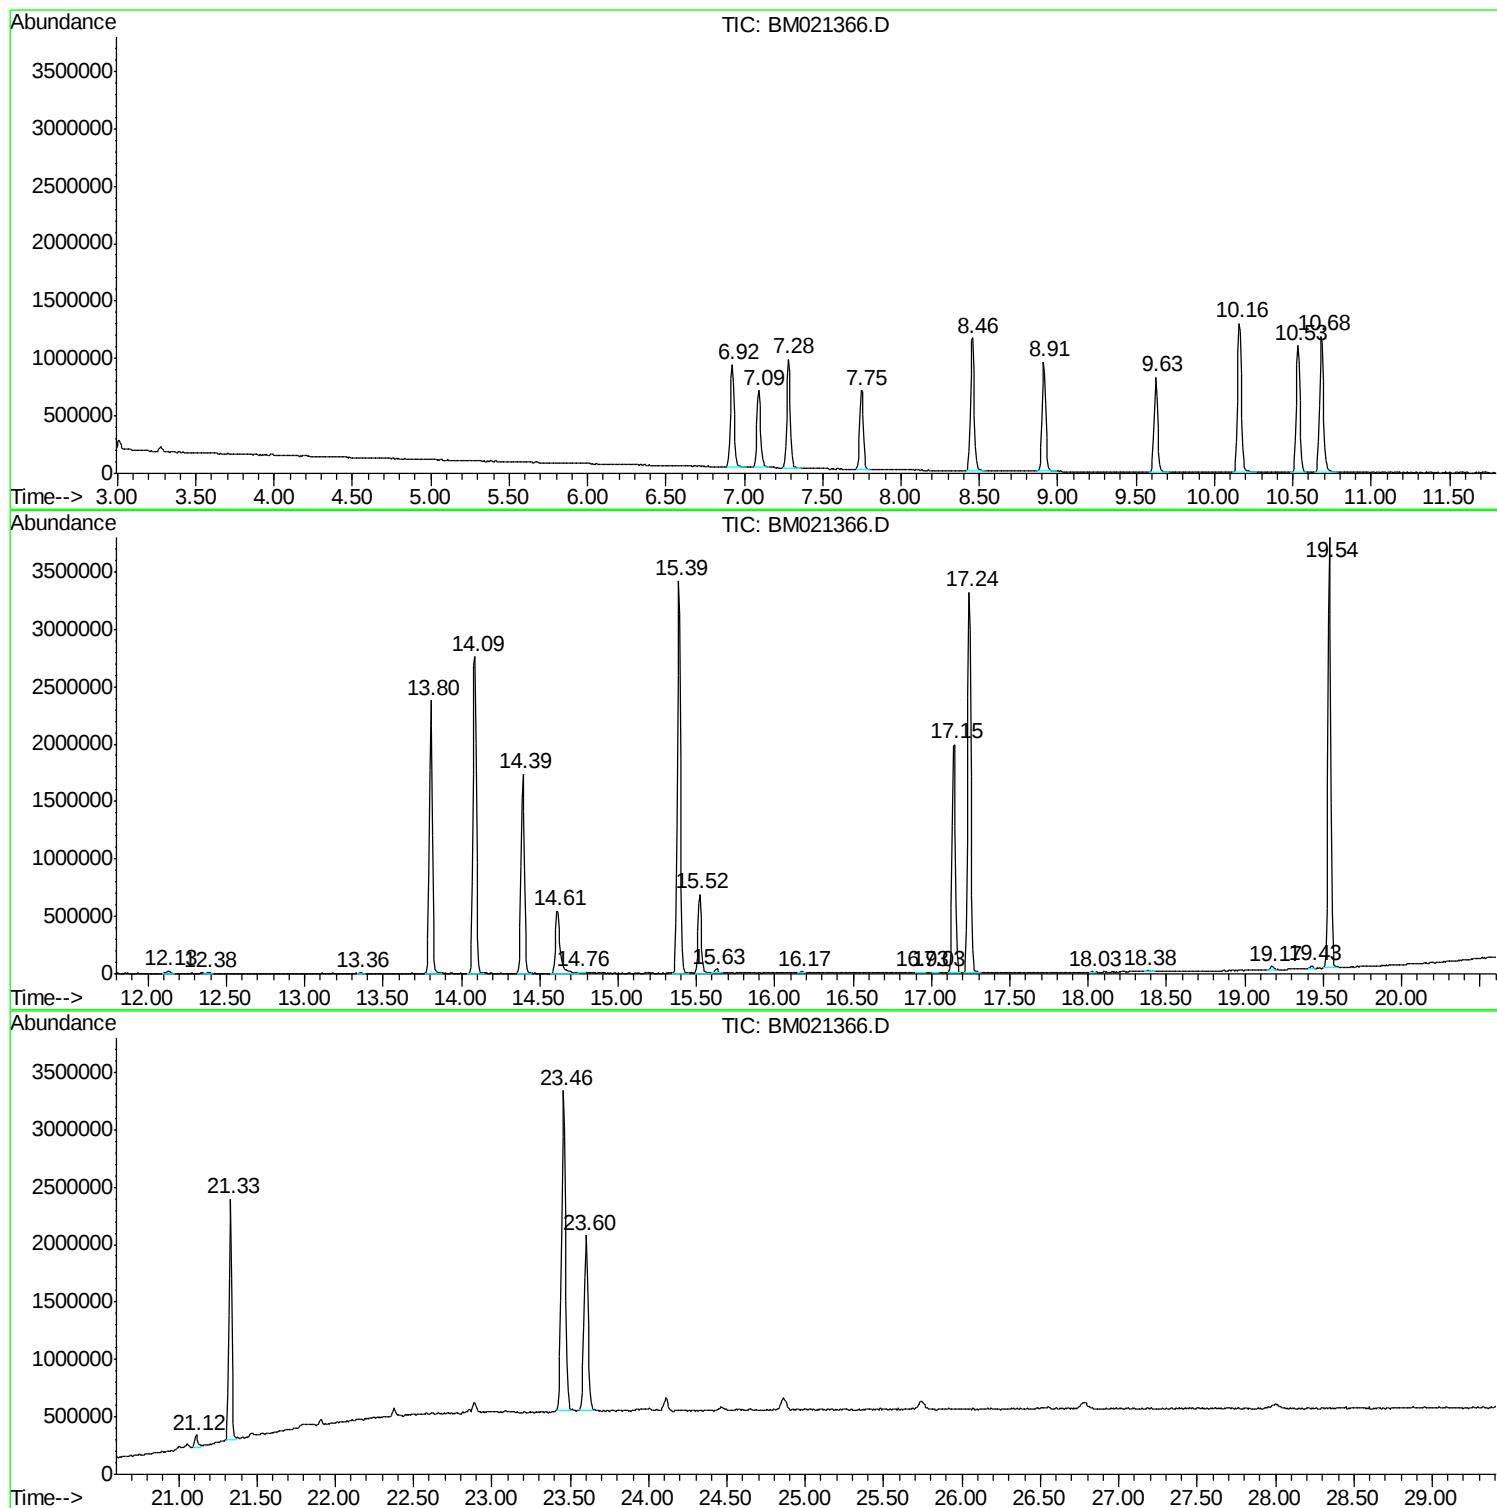

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070319\
Data File : BM021366.D
Acq On : 03 Jul 2019 15:12
Operator : HP/JU
Sample : PB121053BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK53

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070319\
Data File : BM021366.D
Acq On : 03 Jul 2019 15:12
Operator : HP/JU
Sample : PB121053BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK53

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc