

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
 Data File : BM021385.D
 Acq On : 04 Jul 2019 02:57
 Operator : HP/JU
 Sample : PB120861BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	46	49	57	rVB2	52084	77868	1.29%	0.119%
2	6.928	663	670	683	rVB	1055577	1730946	28.63%	2.655%
3	7.087	692	697	707	rVB	808982	1284526	21.25%	1.970%
4	7.281	724	730	741	rVB	1157202	1828497	30.25%	2.804%
5	7.745	803	809	817	rVB	768499	1200580	19.86%	1.841%
6	8.457	923	930	949	rVB	1405078	2323160	38.43%	3.563%
7	8.910	999	1007	1016	rBV	1131055	1867168	30.89%	2.864%
8	9.622	1121	1128	1139	rBV	967894	1619991	26.80%	2.485%
9	10.157	1212	1219	1236	rBV	1558996	2665931	44.10%	4.089%
10	10.534	1275	1283	1290	rBV	1133261	1875634	31.03%	2.877%
11	10.681	1300	1308	1329	rBV	1387530	2478684	41.00%	3.802%
12	12.128	1548	1554	1561	rBV	28806	44794	0.74%	0.069%
13	13.804	1832	1839	1851	rBV	2845228	3981014	65.85%	6.106%
14	14.080	1879	1886	1899	rBV	3392185	4906806	81.17%	7.526%
15	14.386	1932	1938	1948	rBV2	1822440	2725508	45.08%	4.180%
16	14.616	1971	1977	1994	rBV	746562	1378392	22.80%	2.114%
17	15.386	2101	2108	2115	rBV	4250893	6045322	100.00%	9.272%
18	15.516	2124	2130	2143	rBV	771788	1077947	17.83%	1.653%
19	15.627	2144	2149	2153	rVB	44155	63085	1.04%	0.097%
20	16.168	2238	2241	2245	rBV3	8519	9621	0.16%	0.015%
21	16.927	2366	2370	2376	rBV3	7412	10709	0.18%	0.016%
22	17.139	2399	2406	2414	rVB2	2131443	2984167	49.36%	4.577%
23	17.239	2416	2423	2435	rBV	4127763	5841153	96.62%	8.959%
24	18.027	2555	2557	2565	rVB6	5452	9650	0.16%	0.015%
25	19.168	2747	2751	2755	rBV	41175	51748	0.86%	0.079%
26	19.421	2791	2794	2798	rVB	29194	34516	0.57%	0.053%
27	19.533	2807	2813	2821	rBV	4168235	5689211	94.11%	8.726%
28	21.327	3112	3118	3126	rBV	2005228	2657273	43.96%	4.076%
29	23.444	3472	3478	3490	rVB	3263260	5931224	98.11%	9.097%
30	23.592	3497	3503	3512	rVB	1461844	2804602	46.39%	4.302%


Sum of corrected areas: 65199727

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070319\
Data File : BM021385.D
Acq On : 04 Jul 2019 02:57
Operator : HP/JU
Sample : PB120861BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK61

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

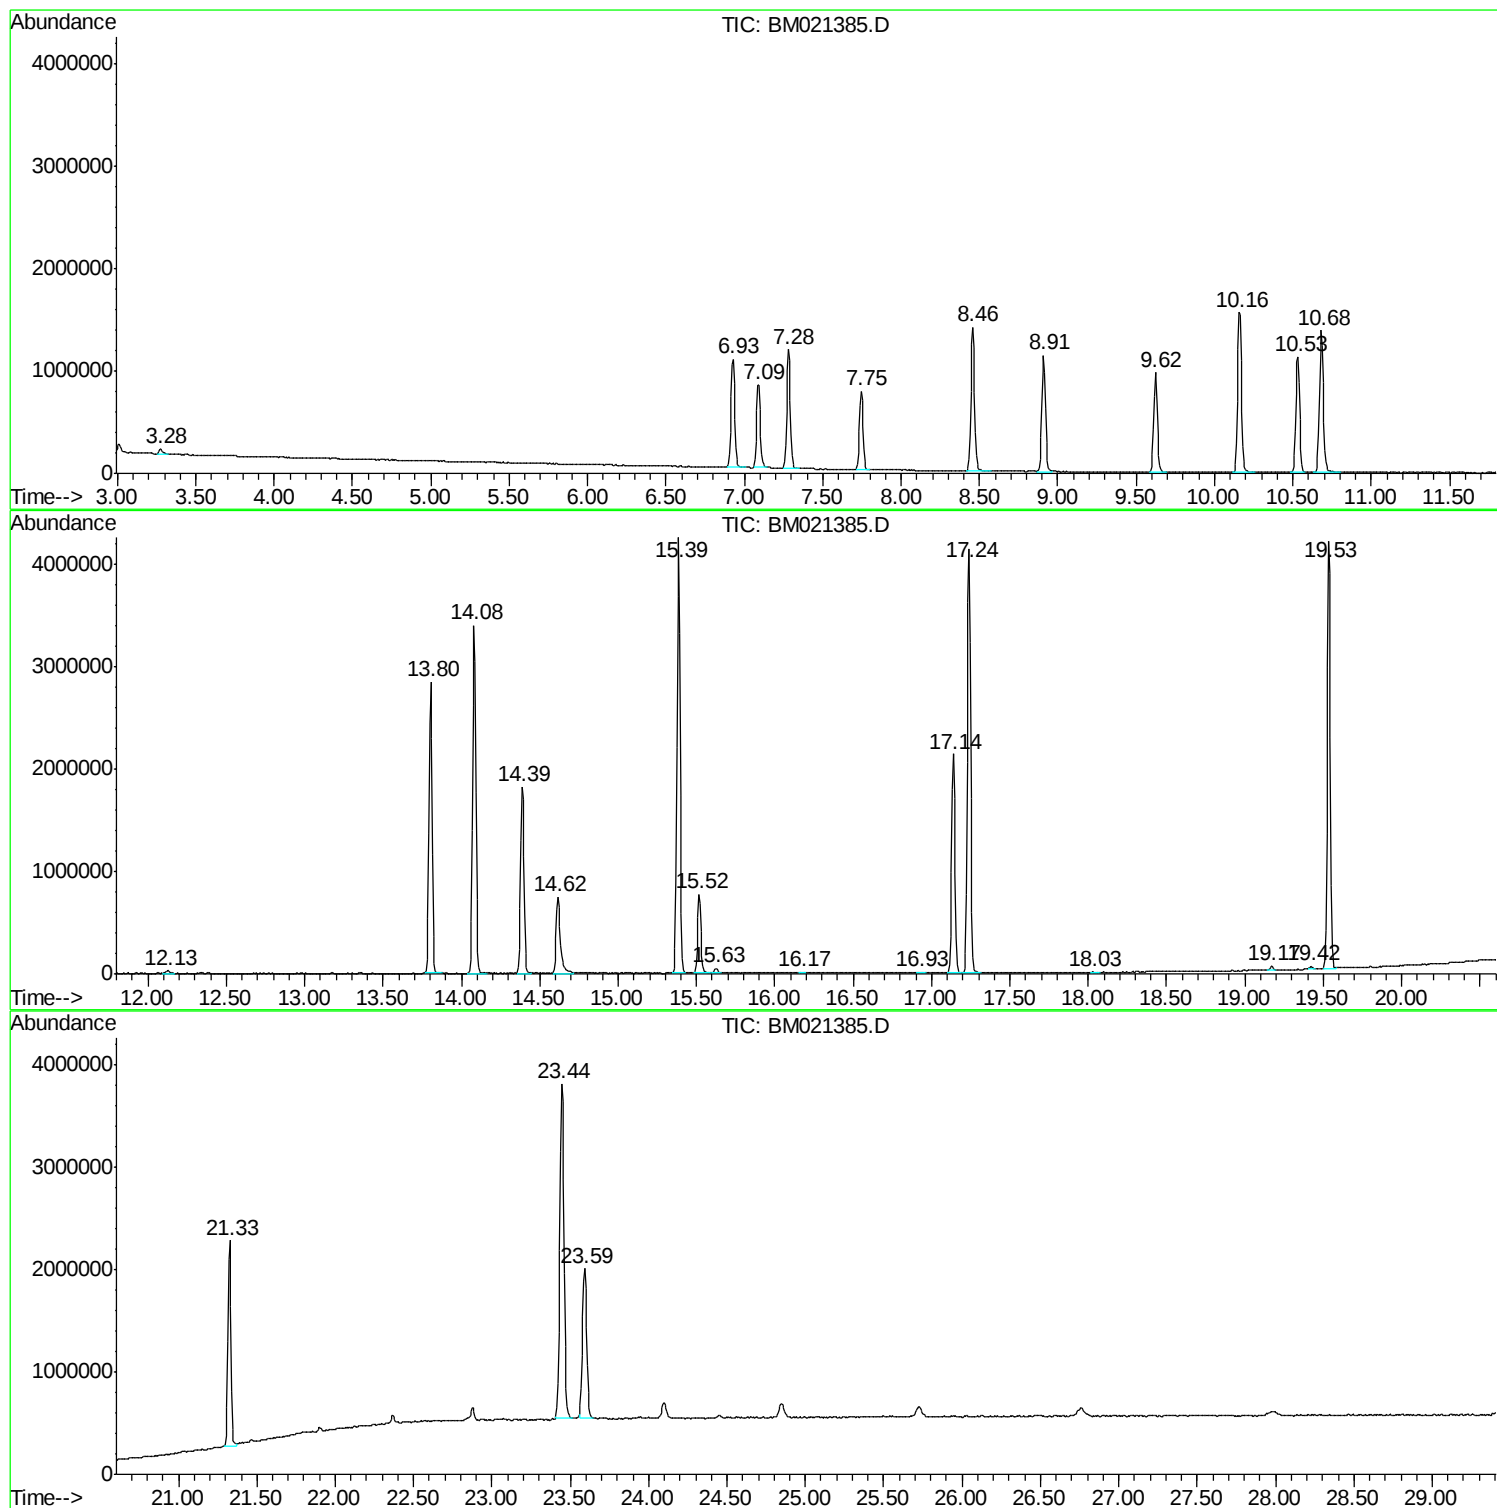

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070319\
Data File : BM021385.D
Acq On : 04 Jul 2019 02:57
Operator : HP/JU
Sample : PB120861BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK61

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070319\
Data File : BM021385.D
Acq On : 04 Jul 2019 02:57
Operator : HP/JU
Sample : PB120861BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK61

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc