

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070323\
 Data File : BM040566.D
 Acq On : 03 Jul 2023 09:16
 Operator : MA/JU
 Sample : PB153767BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK767

Quant Time: Jul 03 13:35:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 03:00:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.923	152	5643	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.728	136	20366	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.568	164	10679	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.315	188	20151	0.400	ng/ul	-0.01
17) Chrysene-d12	21.506	240	12347	0.400	ng/ul	0.00
23) Perylene-d12	23.914	264	14237	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.316	96	40269	4.543	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.323	152	8205	0.287	ng/ul	-0.01
18) Fluoranthene-d10	19.347	212	12461	0.315	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.562	166	2908	0.068	ng/ul#	16
20) Pyrene	19.709	202	1983	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.759	252	3635	0.073	ng/ul#	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070323\
Data File : BM040566.D
Acq On : 03 Jul 2023 09:16
Operator : MA/JU
Sample : PB153767BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK767

Quant Time: Jul 03 13:35:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 03:00:05 2023
Response via : Initial Calibration




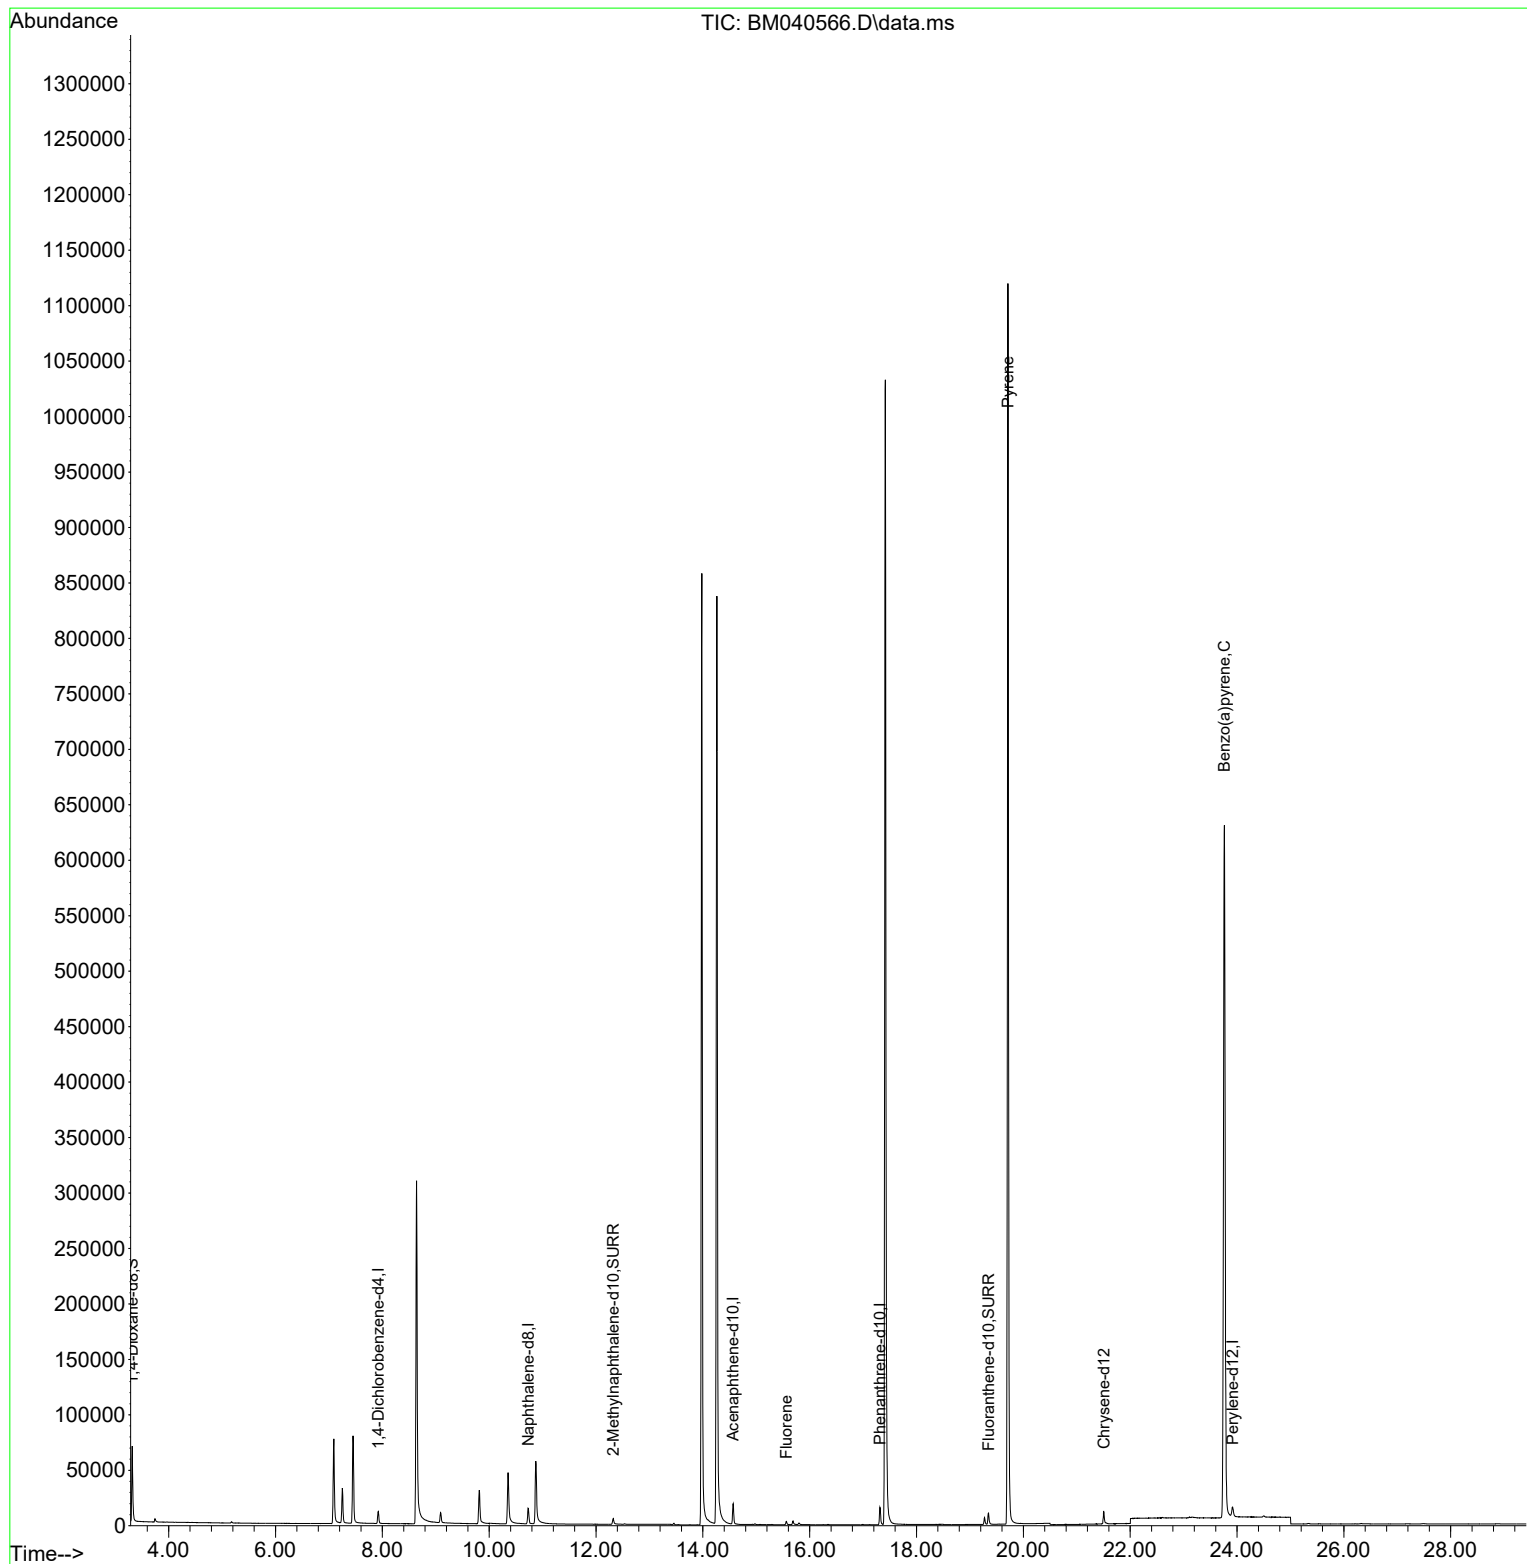


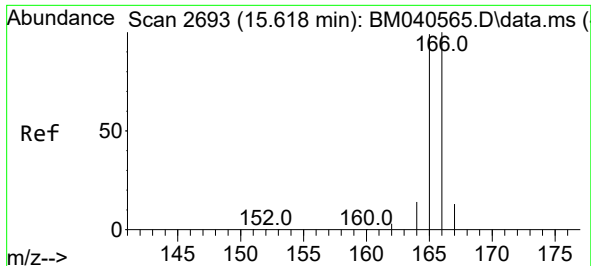

#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.562 min Scan# 20
Delta R.T. -0.069 min
Lab File: BM040566.D
Acq: 03 Jul 2023 09:16




Instrument :
BNA_M
ClientSampleId :
SBLK767


Tgt Ion:166 Resp: 2908
Ion Ratio Lower Upper
166 100
165 11.2 79.6 119.4#
167 35.2 11.4 17.0#

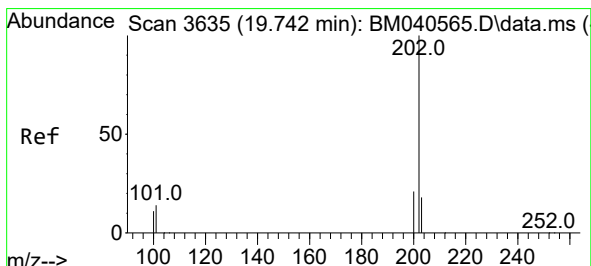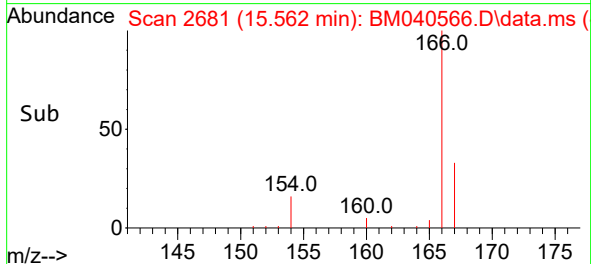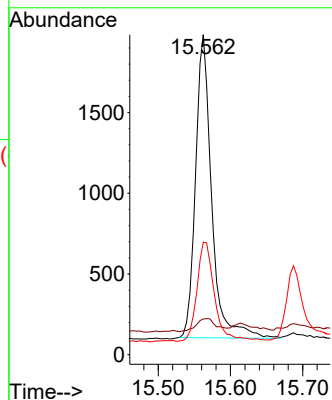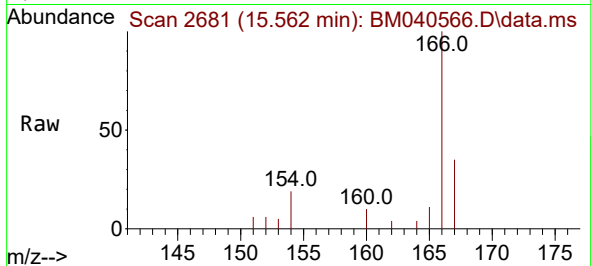

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.709 min Scan# 3628
Delta R.T. -0.037 min
Lab File: BM040566.D
Acq: 03 Jul 2023 09:16


Tgt Ion:202 Resp: 1983
Ion Ratio Lower Upper
202 100
101 172.9 12.6 18.8#
100 1281.2 9.8 14.6#

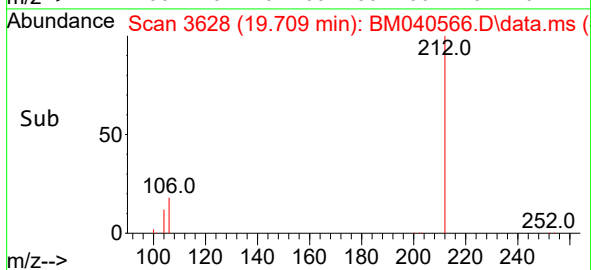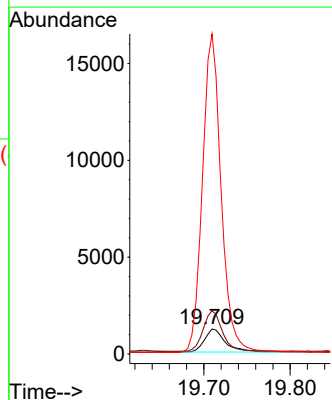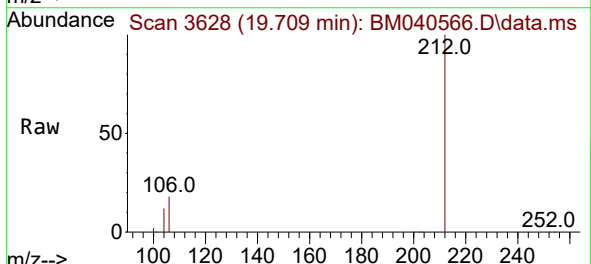

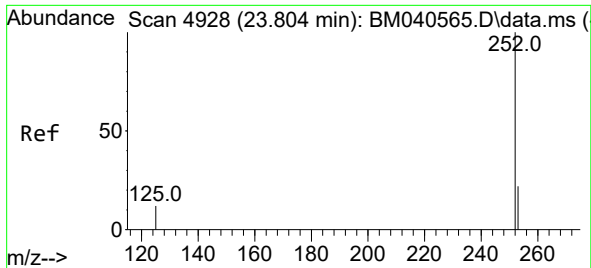

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.759 min Scan# 4913
Delta R.T. -0.053 min
Lab File: BM040566.D
Acq: 03 Jul 2023 09:16

Instrument :
BNA_M
ClientSampleId :
SBLK767

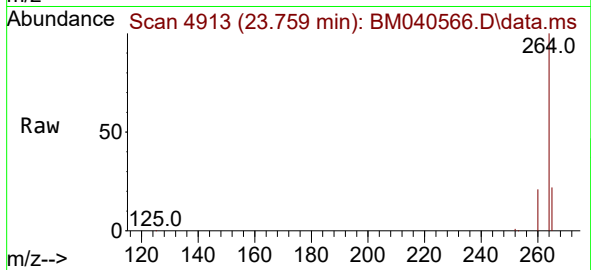

Tgt Ion:252 Resp: 3635
Ion Ratio Lower Upper
252 100
253 66.1 22.9 34.3#
125 80.1 21.0 31.4#

