

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070323\
 Data File : BM040583.D
 Acq On : 03 Jul 2023 20:01
 Operator : MA/JU
 Sample : PB153508BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK508

Quant Time: Jul 04 01:30:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 03 13:40:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.923	152	6256	0.400	ng/ul	0.00
4) Naphthalene-d8	10.728	136	22797	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.568	164	11669	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.315	188	20845	0.400	ng/ul	0.00
17) Chrysene-d12	21.503	240	12431	0.400	ng/ul	0.00
23) Perylene-d12	23.914	264	15412	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.316	96	44715	4.550	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.318	152	9332	0.292	ng/ul	0.00
18) Fluoranthene-d10	19.342	212	12890	0.323	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.562	166	3236	0.069	ng/ul#	16
20) Pyrene	19.709	202	2114	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.757	252	3927	0.073	ng/ul#	21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070323\
Data File : BM040583.D
Acq On : 03 Jul 2023 20:01
Operator : MA/JU
Sample : PB153508BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK508

Quant Time: Jul 04 01:30:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 03 13:40:38 2023
Response via : Initial Calibration




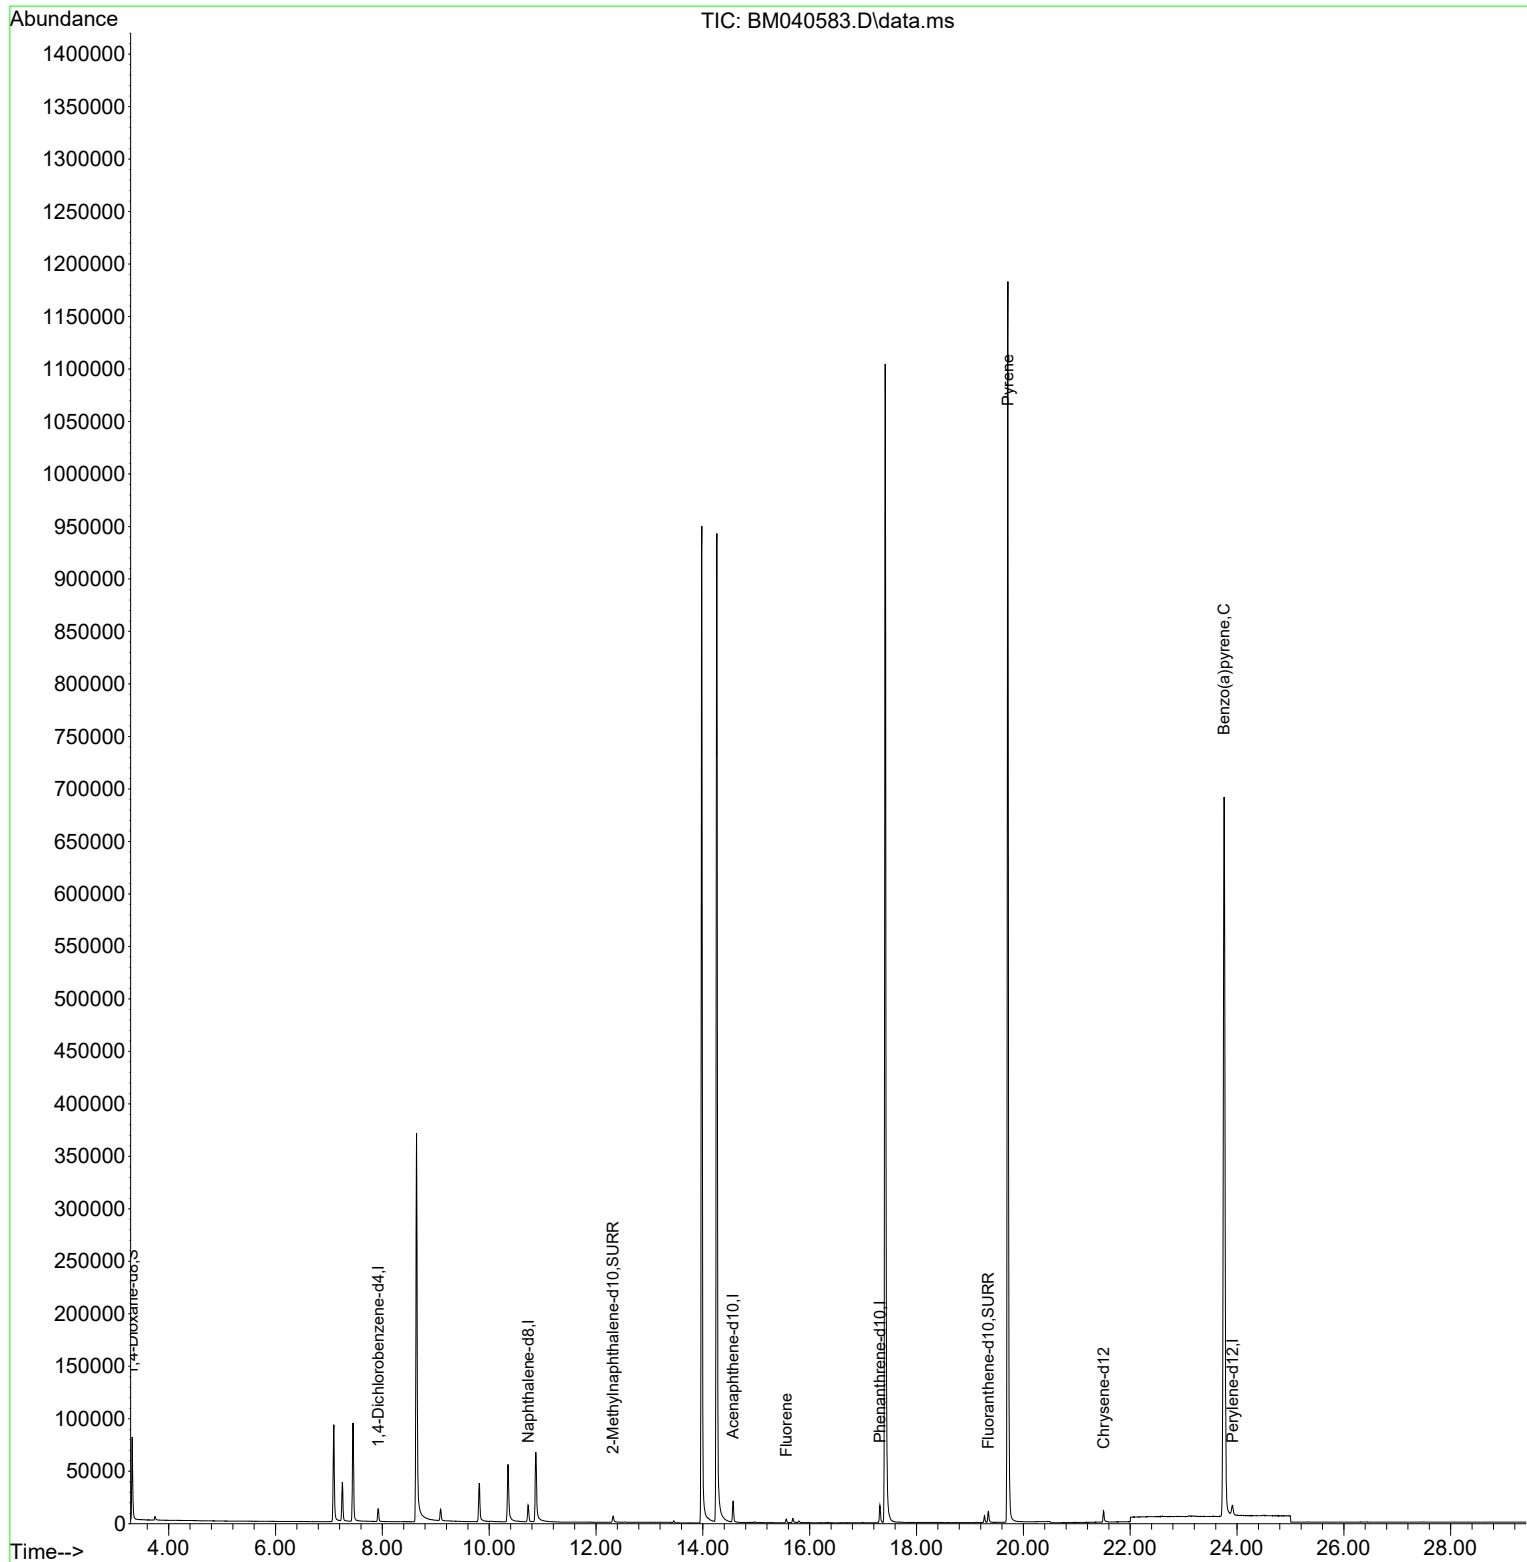


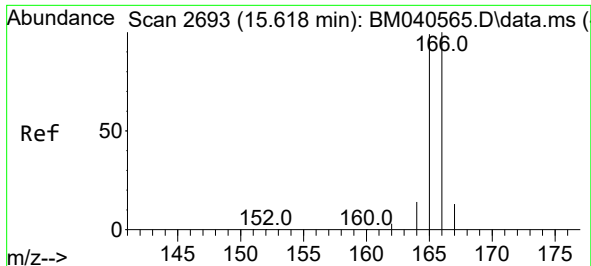

#12
Fluorene
Concen: 0.069 ng/ul
RT: 15.562 min Scan# 2
Delta R.T. -0.056 min
Lab File: BM040583.D
Acq: 03 Jul 2023 20:01




Instrument :
BNA_M
ClientSampleId :
SBLK508


Tgt Ion:166 Resp: 3236
Ion Ratio Lower Upper
166 100
165 11.2 79.6 119.4#
167 34.0 11.4 17.0#

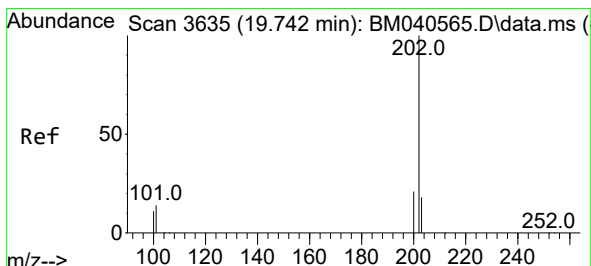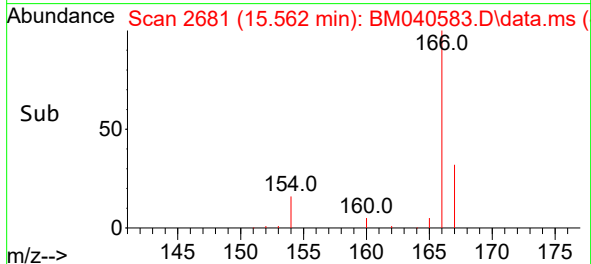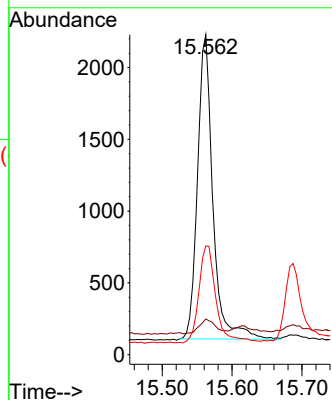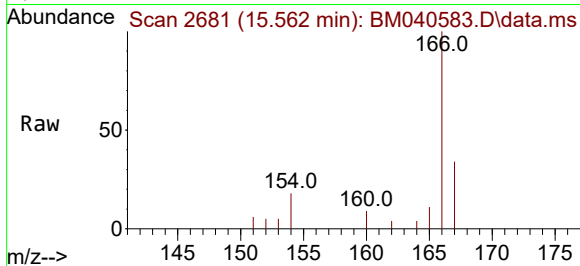

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.709 min Scan# 3628
Delta R.T. -0.033 min
Lab File: BM040583.D
Acq: 03 Jul 2023 20:01


Tgt Ion:202 Resp: 2114
Ion Ratio Lower Upper
202 100
101 169.8 12.6 18.8#
100 1222.9 9.8 14.6#

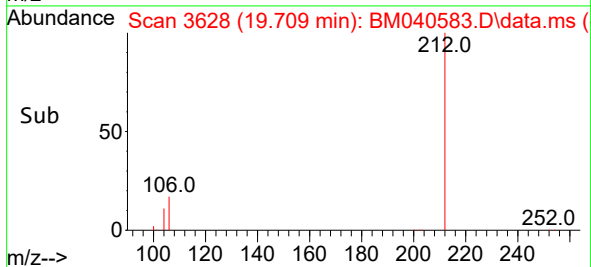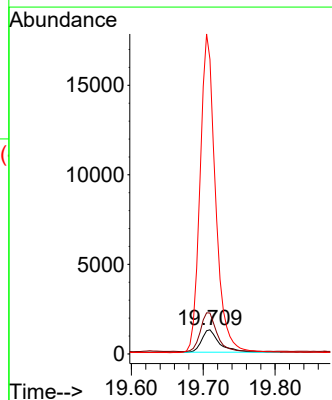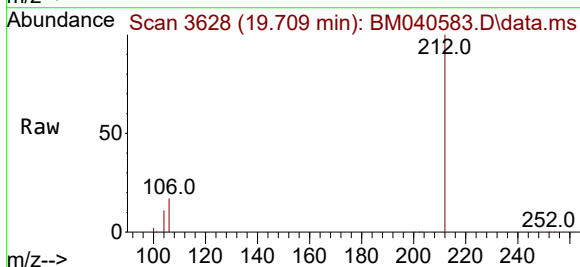

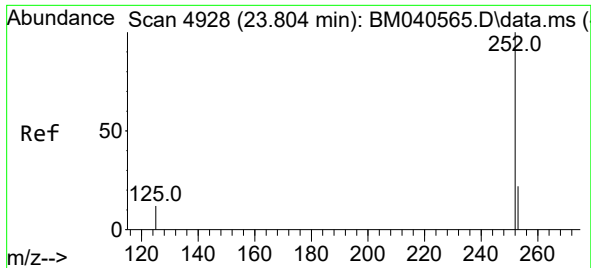

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.757 min Scan# 4912
Delta R.T. -0.047 min
Lab File: BM040583.D
Acq: 03 Jul 2023 20:01

Instrument :
BNA_M
ClientSampleId :
SBLK508

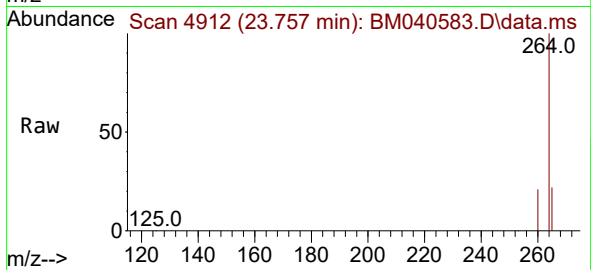

Tgt Ion:252 Resp: 3927
Ion Ratio Lower Upper
252 100
253 65.1 22.9 34.3#
125 72.1 21.0 31.4#

