

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070323\
 Data File : BM040602.D
 Acq On : 04 Jul 2023 08:29
 Operator : MA/JU
 Sample : PB153767BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 05 01:16:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 03 13:40:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.915	152	6691	0.400	ng/ul	0.00
4) Naphthalene-d8	10.723	136	24287	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.559	164	12483	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.307	188	22777	0.400	ng/ul	-0.01
17) Chrysene-d12	21.497	240	12677	0.400	ng/ul	0.00
23) Perylene-d12	23.900	264	14376	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.312	96	52091	4.956	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.312	152	10249	0.301	ng/ul	-0.01
18) Fluoranthene-d10	19.338	212	13208	0.325	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.553	166	3593	0.071	ng/ul#	15
20) Pyrene	19.700	202	2224	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.748	252	4050	0.081	ng/ul#	20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070323\
Data File : BM040602.D
Acq On : 04 Jul 2023 08:29
Operator : MA/JU
Sample : PB153767BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 05 01:16:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 03 13:40:38 2023
Response via : Initial Calibration




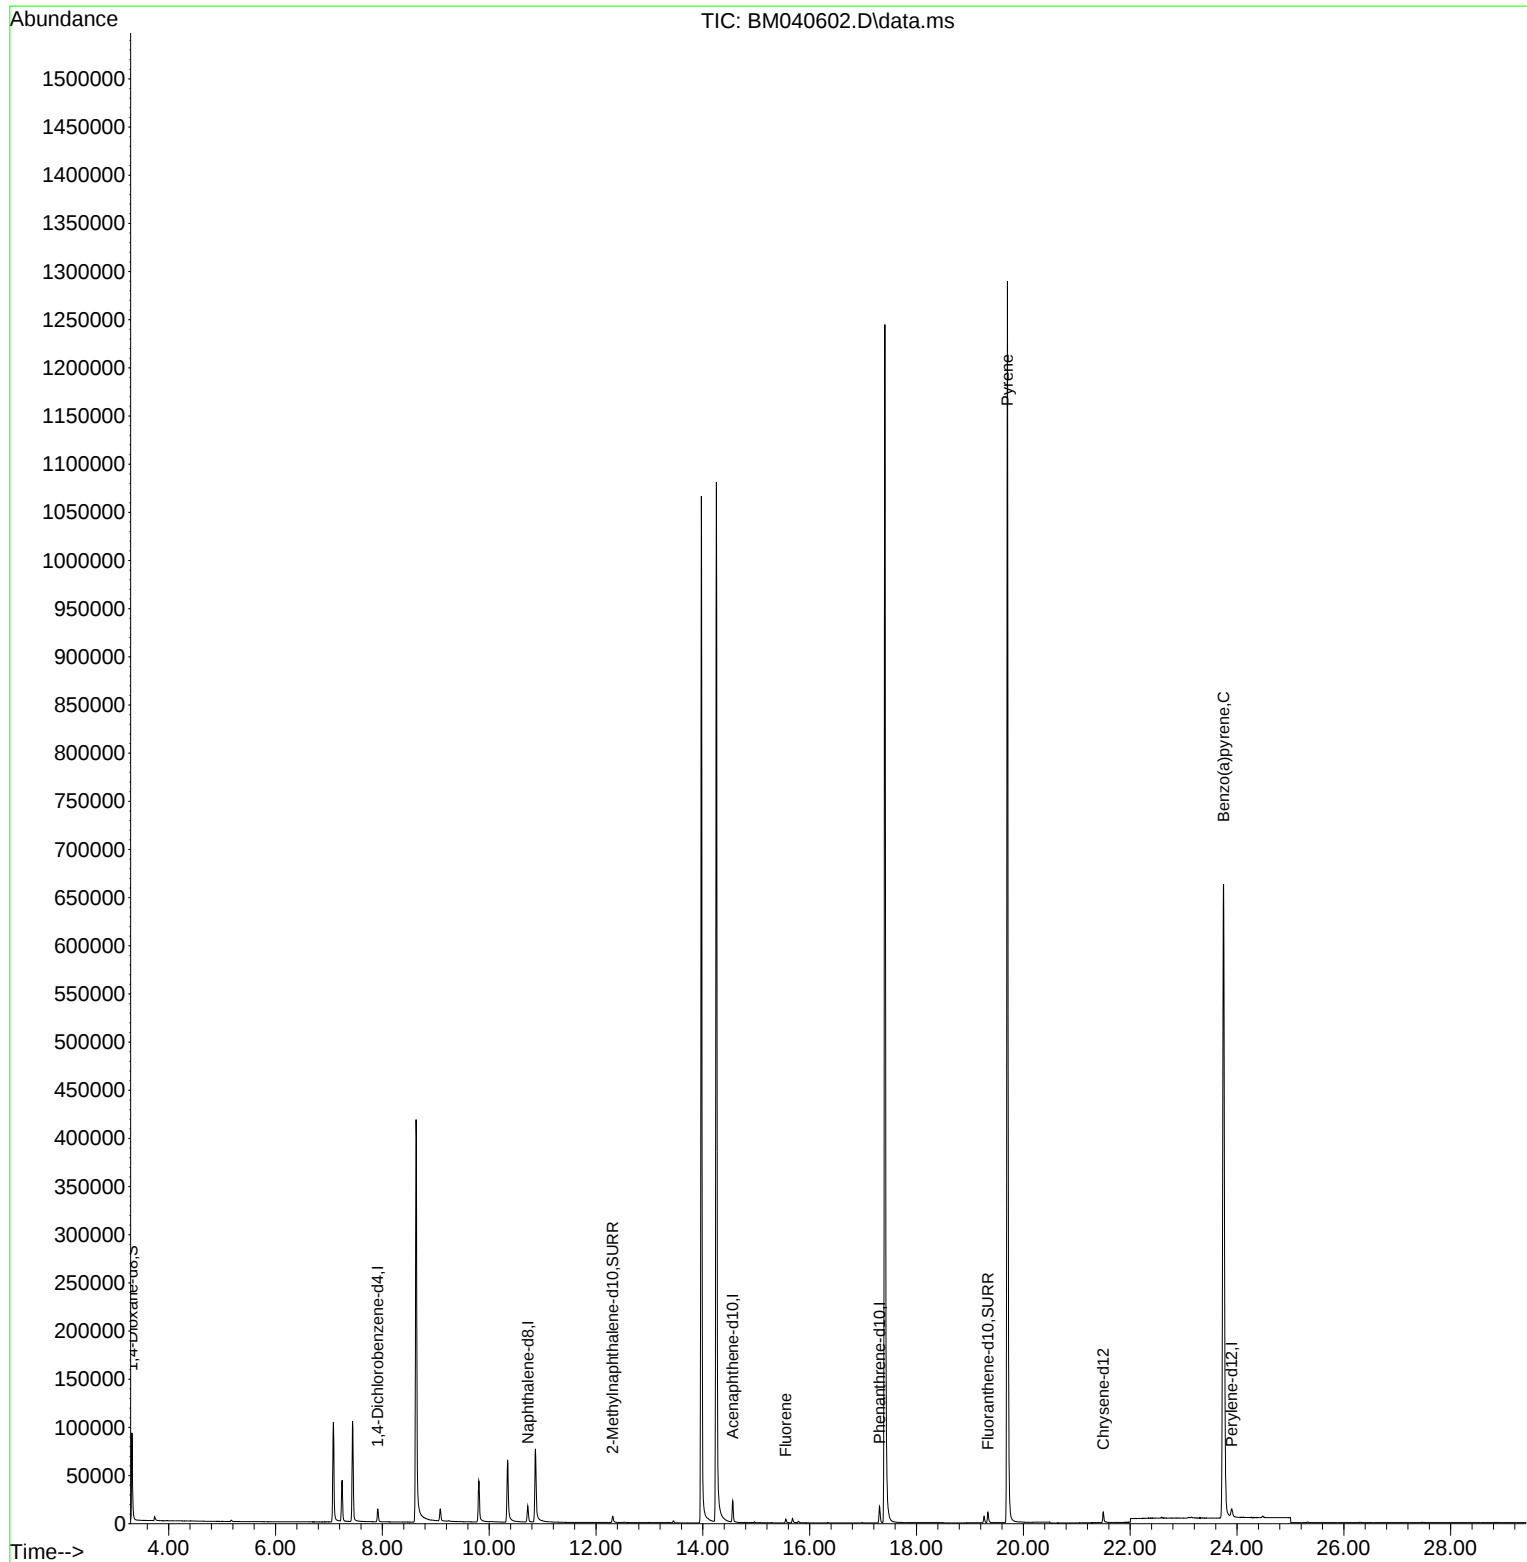


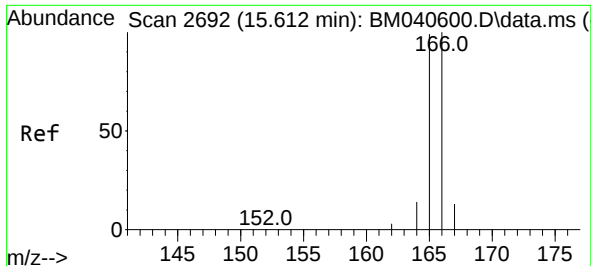

#12
Fluorene
Concen: 0.071 ng/ul
RT: 15.553 min Scan# 20
Delta R.T. -0.065 min
Lab File: BM040602.D
Acq: 04 Jul 2023 08:29




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:166 Resp: 3593
Ion Ratio Lower Upper
166 100
165 9.7 79.6 119.4#
167 33.4 11.4 17.0#

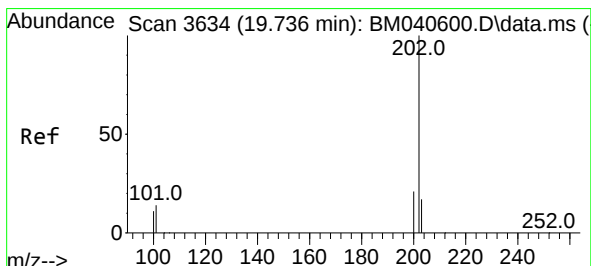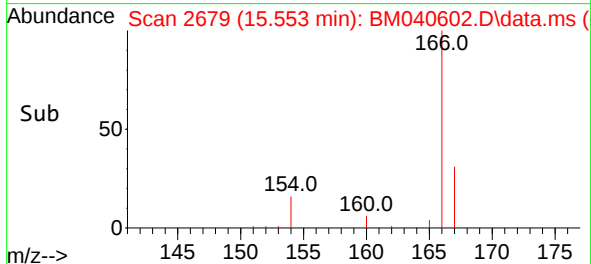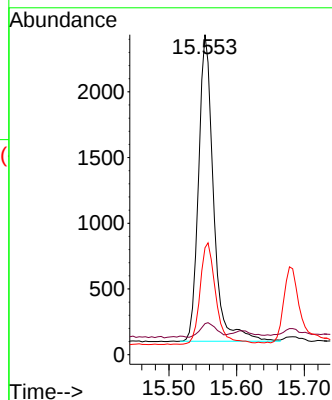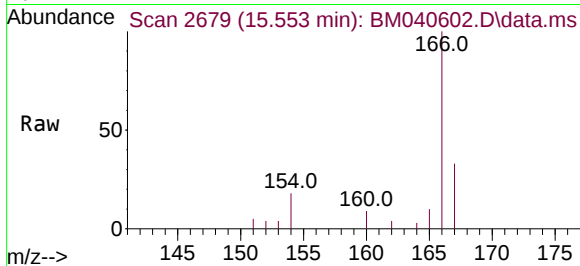

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.700 min Scan# 3626
Delta R.T. -0.042 min
Lab File: BM040602.D
Acq: 04 Jul 2023 08:29


Tgt Ion:202 Resp: 2224
Ion Ratio Lower Upper
202 100
101 176.2 12.6 18.8#
100 1354.1 9.8 14.6#

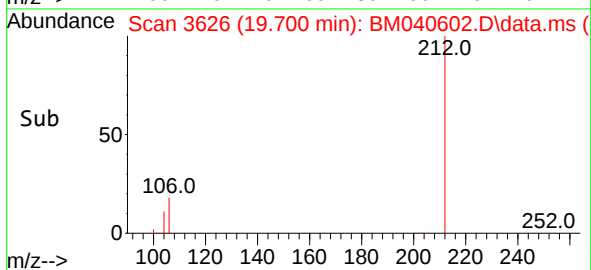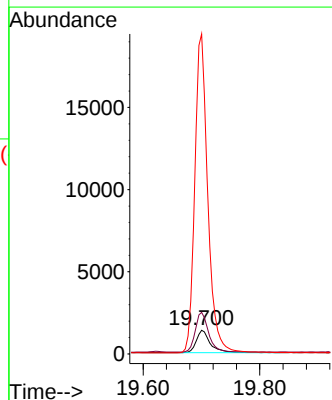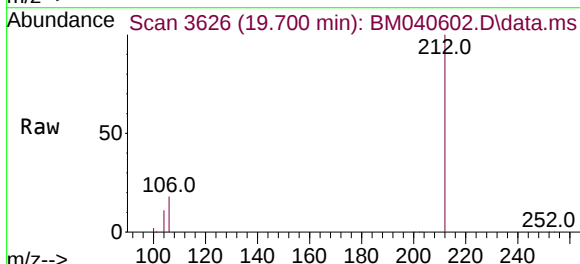

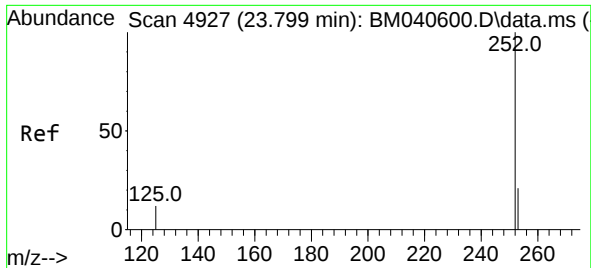

#26
 Benzo(a)pyrene
 Concen: 0.081 ng/ul
 RT: 23.748 min Scan# 4909
 Delta R.T. -0.056 min
 Lab File: BM040602.D
 Acq: 04 Jul 2023 08:29

Instrument :
 BNA_M
 ClientSampleId :

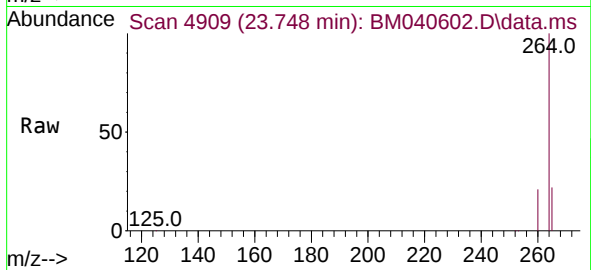

Tgt Ion:252 Resp: 4050
 Ion Ratio Lower Upper
 252 100
 253 59.5 22.9 34.3#
 125 79.8 21.0 31.4#

