
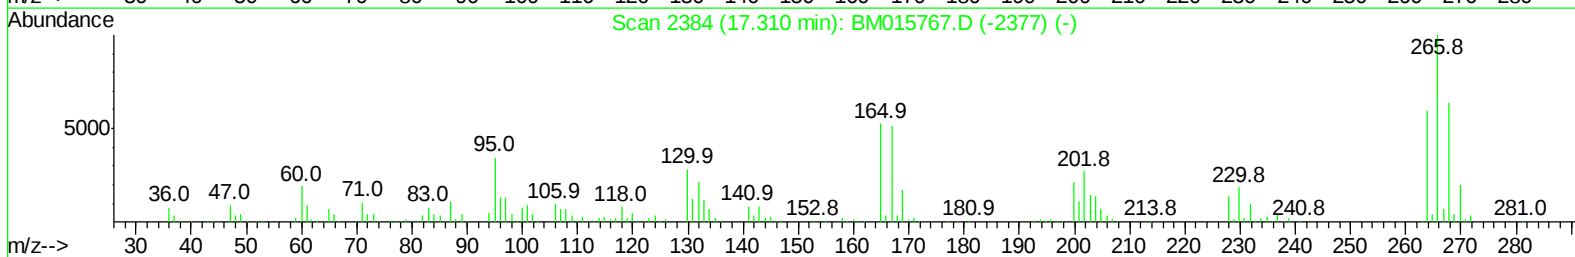
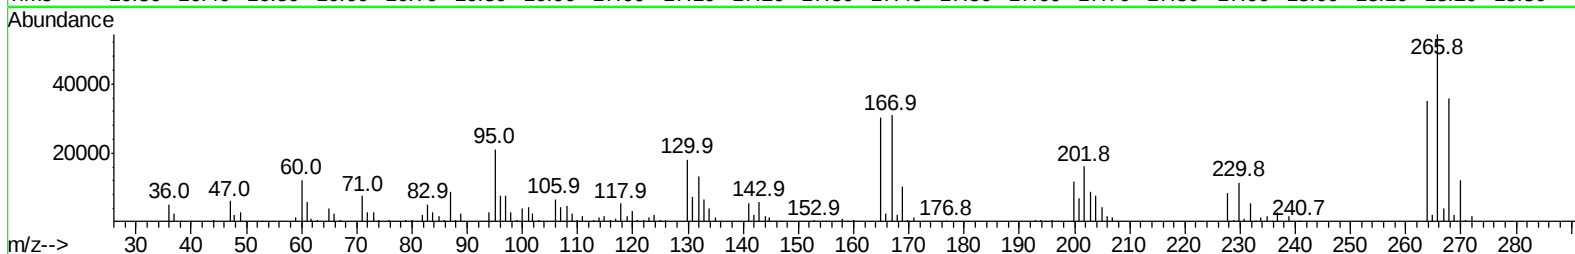


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070518\
Data File : BM015763.D
Acq On : 05 Jul 2018 12:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 07:56:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 05 17:39:50 2018
Response via : Initial Calibration

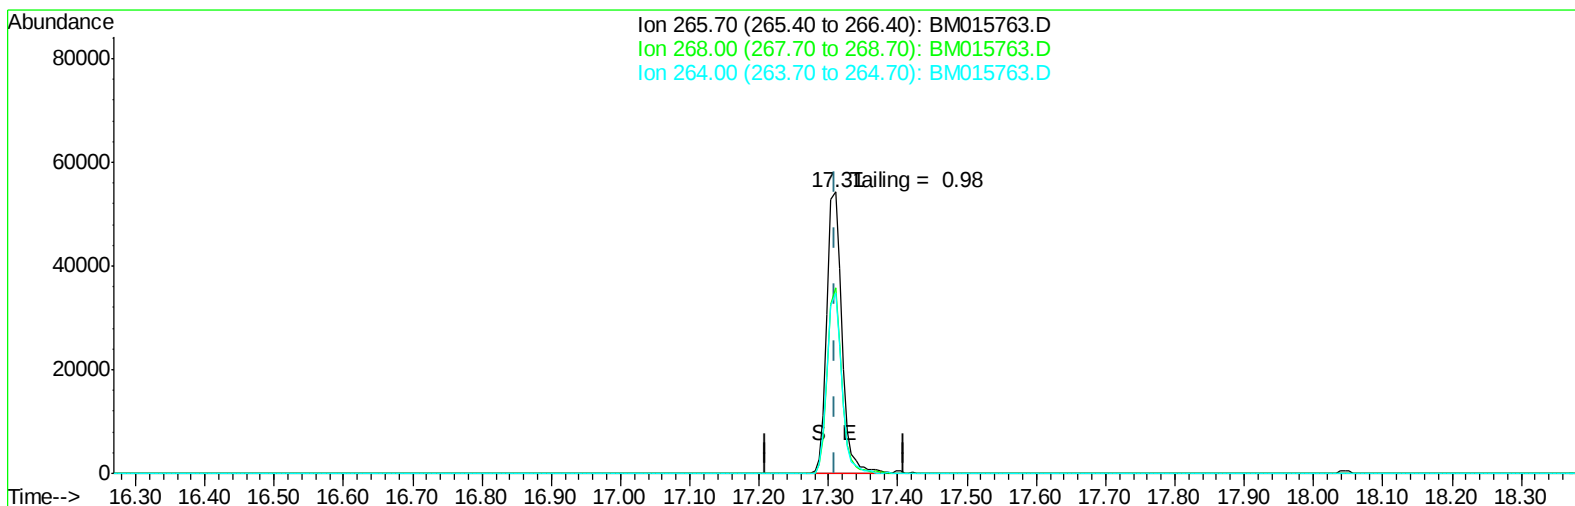

TIC: BM015763.D

(69) Pentachlorophenol (C)




17.310min (-0.000) 0.00ng

response 81591

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	65.98
264.00	61.20	64.29
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070518\
Data File : BM015763.D
Acq On : 05 Jul 2018 12:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 07:56:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 05 17:39:50 2018
Response via : Initial Calibration

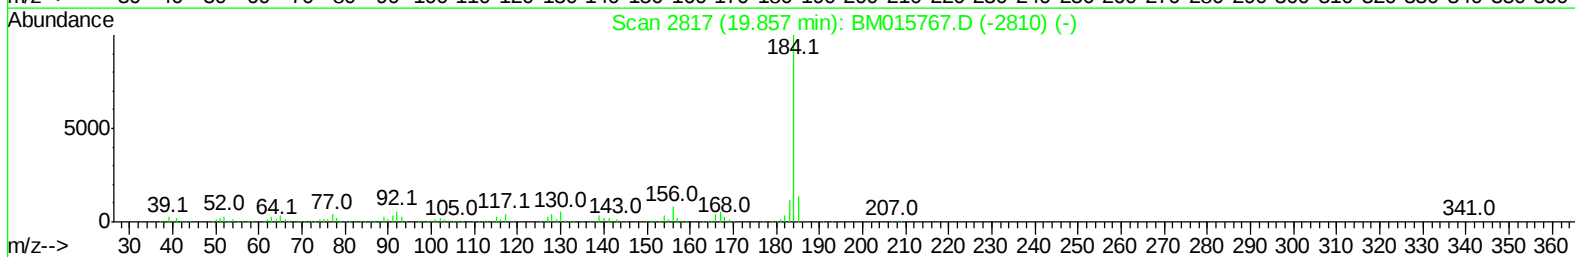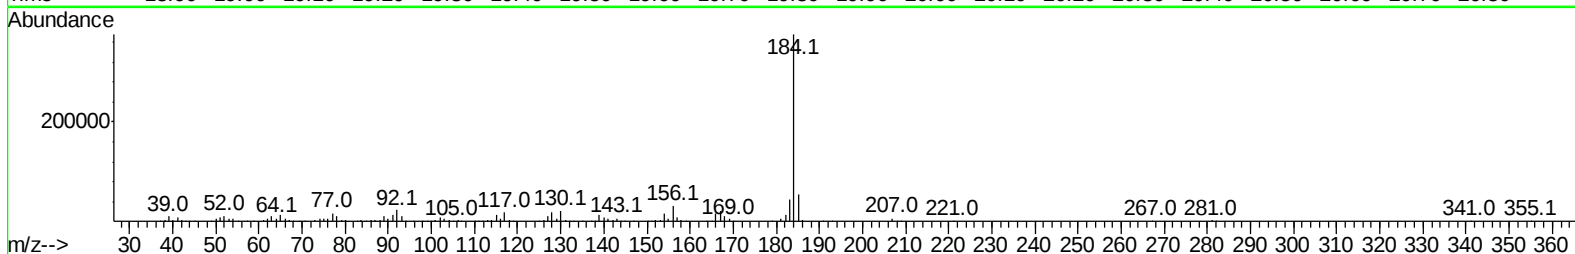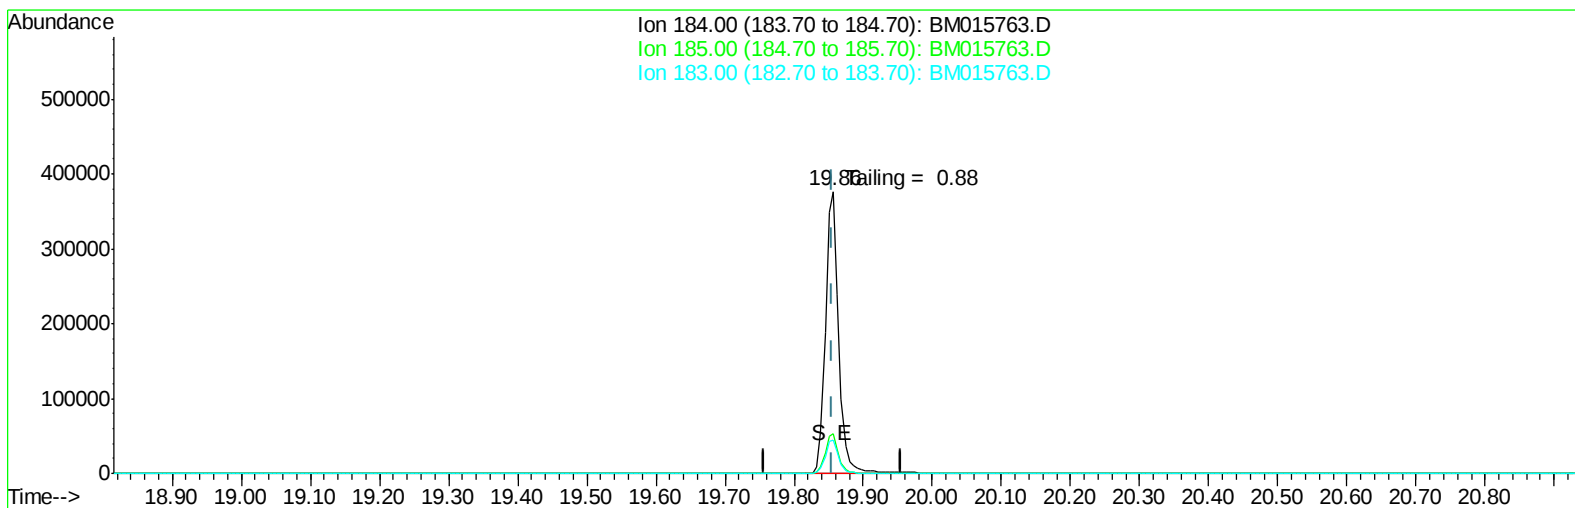

TIC: BM015763.D

(76) Benzidine

19.857min (-0.000) 2485.79ng

response 495761

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.19
183.00	11.10	11.85
0.00	0.00	0.00