

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070518\
 Data File : BM015802.D
 Acq On : 06 Jul 2018 15:13
 Operator : SJ/JU
 Sample : PB110837BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB110837BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.328	342	347	359	rBV	379344	574741	6.47%	1.037%
2	5.810	423	429	447	rBV	3689091	5471269	61.59%	9.874%
3	7.463	702	710	725	rBV	3590736	5844135	65.79%	10.547%
4	7.834	766	773	788	rBV	3896364	6200754	69.81%	11.190%
5	8.304	847	853	866	rBV	545622	908003	10.22%	1.639%
6	8.634	902	909	925	rBV	2798272	4436398	49.94%	8.006%
7	9.498	1048	1056	1070	rBV	2121627	3537971	39.83%	6.385%
8	11.133	1327	1334	1344	rBV	662725	1131398	12.74%	2.042%
9	13.557	1739	1746	1756	rBV	5455714	7638155	85.99%	13.784%
10	14.927	1973	1979	1989	rBV2	918081	1382854	15.57%	2.496%
11	16.410	2224	2231	2251	rBV	4341701	5922628	66.67%	10.688%
12	17.651	2436	2442	2451	rBV	1045595	1474588	16.60%	2.661%
13	20.215	2872	2878	2883	rBV	7819969	8882878	100.00%	16.030%
14	21.762	3136	3141	3152	rBV	866708	1141884	12.85%	2.061%
15	24.168	3544	3550	3559	rVB	441259	865063	9.74%	1.561%


Sum of corrected areas: 55412719

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070518\
Data File : BM015802.D
Acq On : 06 Jul 2018 15:13
Operator : SJ/JU
Sample : PB110837BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB110837BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

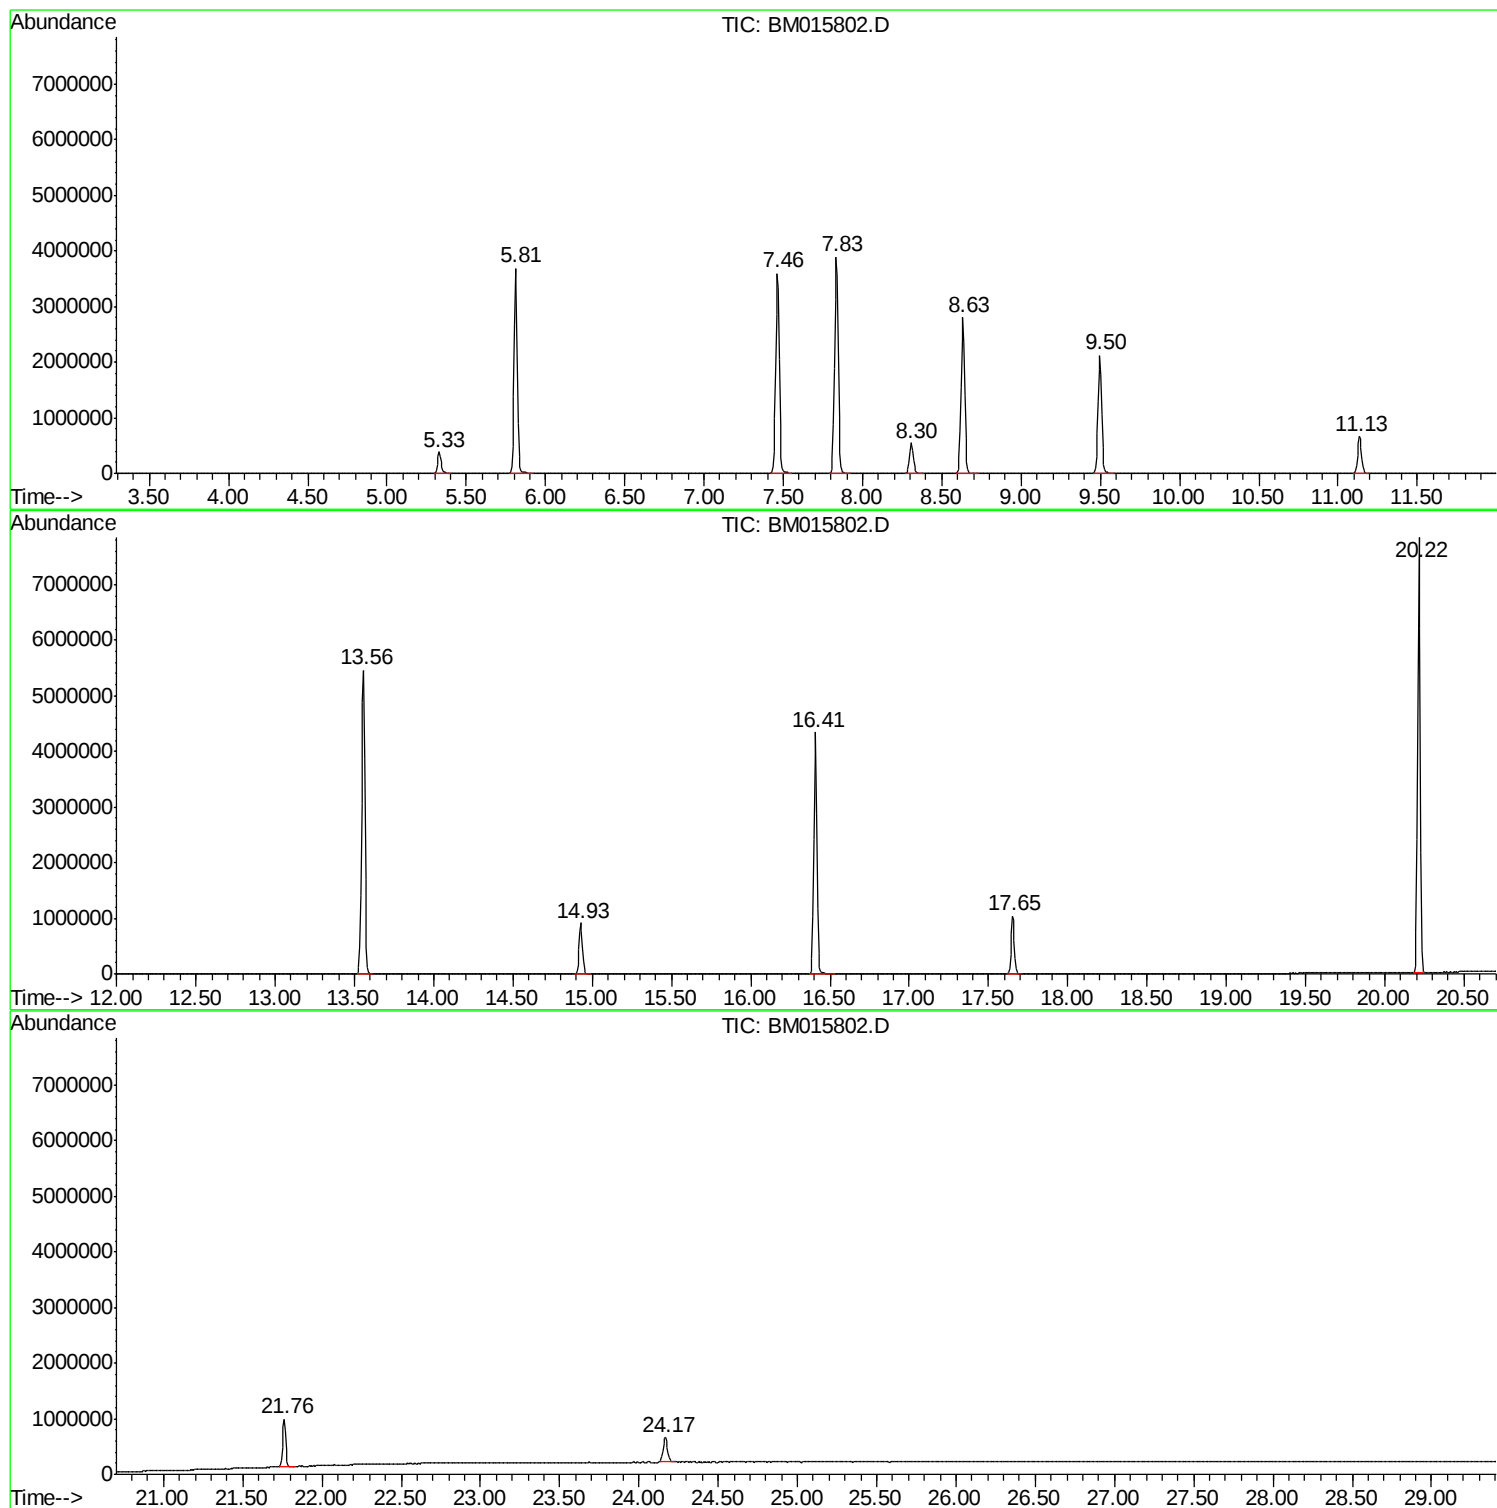

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070518\
Data File : BM015802.D
Acq On : 06 Jul 2018 15:13
Operator : SJ/JU
Sample : PB110837BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB110837BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.33 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.33	12.66 ng	574741	1,4-Dichlorobenzene-d4	8.30

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45
2		Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	38
3		1-Butene, 4-ethoxy-	100	C6H12O	044611-46-3	23
4		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16
5		Butane	58	C4H10	000106-97-8	9

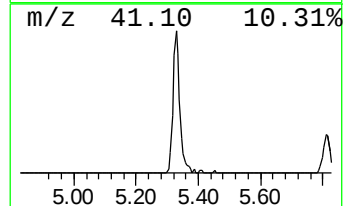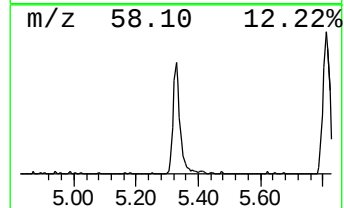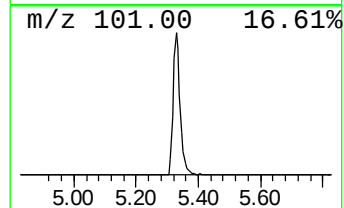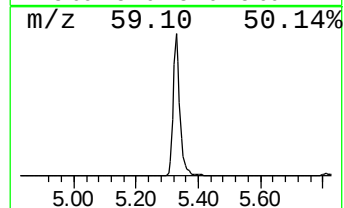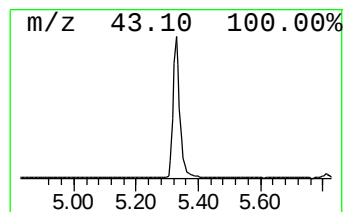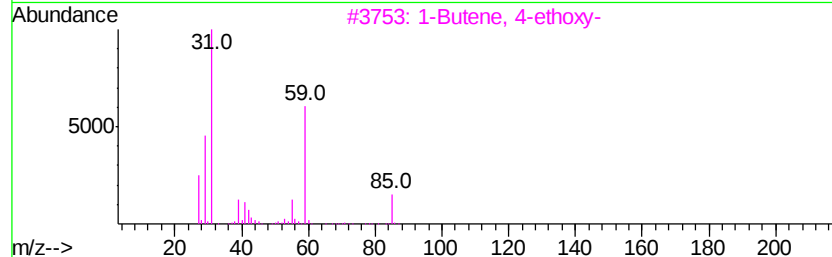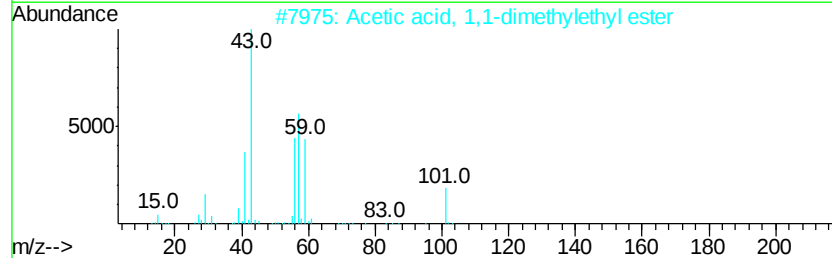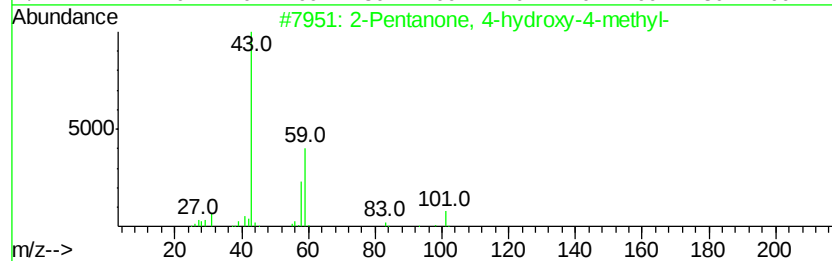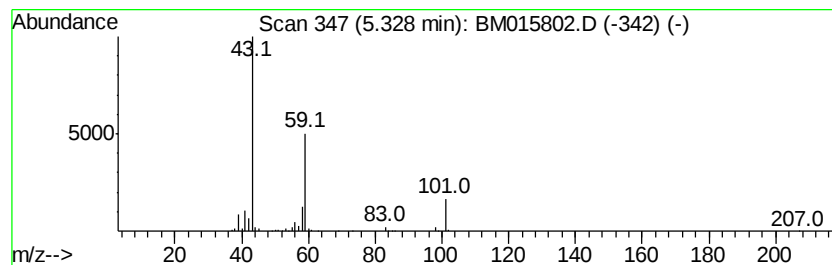

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070518\
Data File : BM015802.D
Acq On : 06 Jul 2018 15:13
Operator : SJ/JU
Sample : PB110837BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB110837BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.83 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.83	136.58 ng	6200750	1,4-Dichlorobenzene-d4	8.30

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	25
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	22
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
5		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16

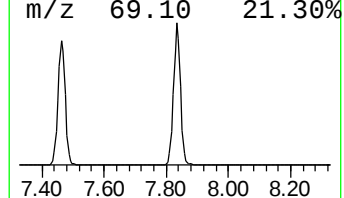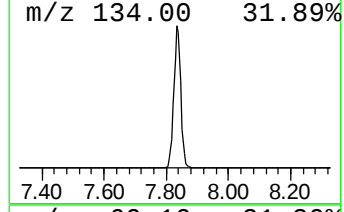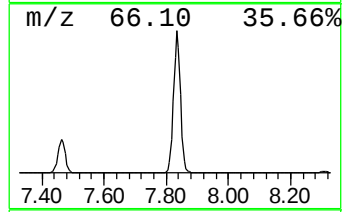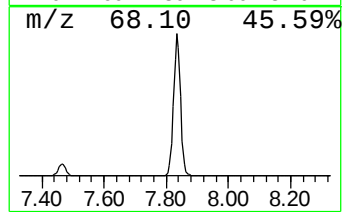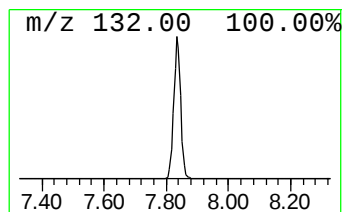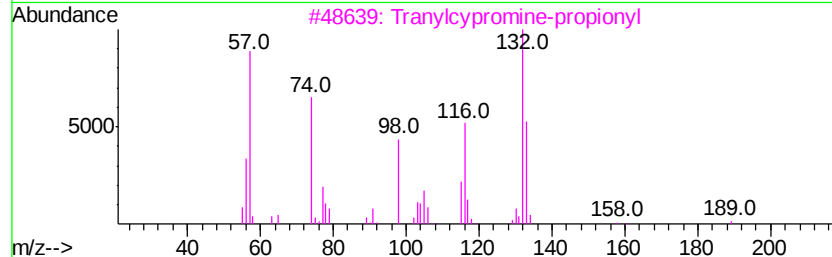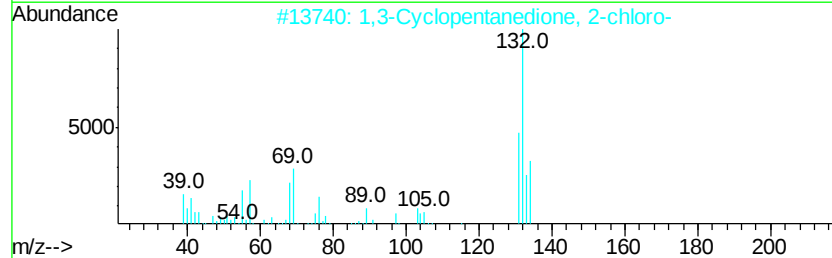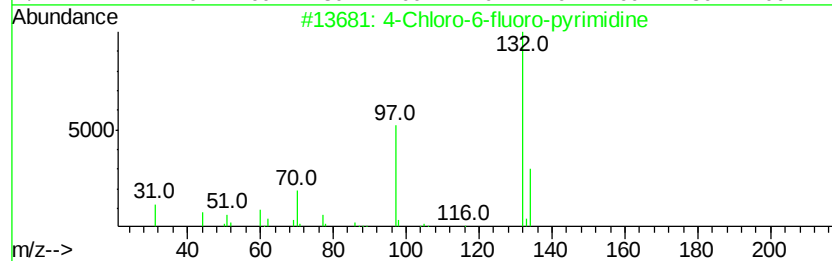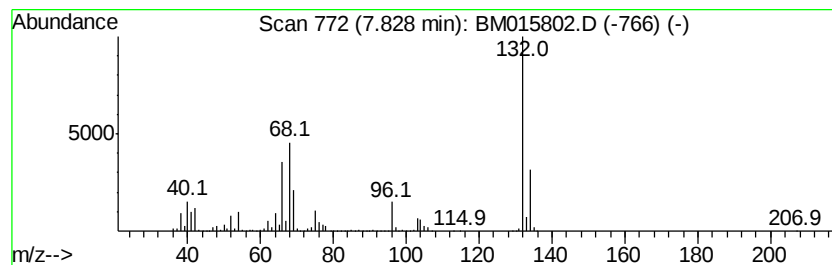

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070518\
Data File : BM015802.D
Acq On : 06 Jul 2018 15:13
Operator : SJ/JU
Sample : PB110837BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB110837BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.33	5.33	12.7	ng	574741	1	8.30	908003	20.0
unknown7.83	7.83	136.6	ng	6200750	1	8.30	908003	20.0