


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070518\
 Data File : BM015763.D
 Acq On : 05 Jul 2018 12:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 05 17:39:50 2018

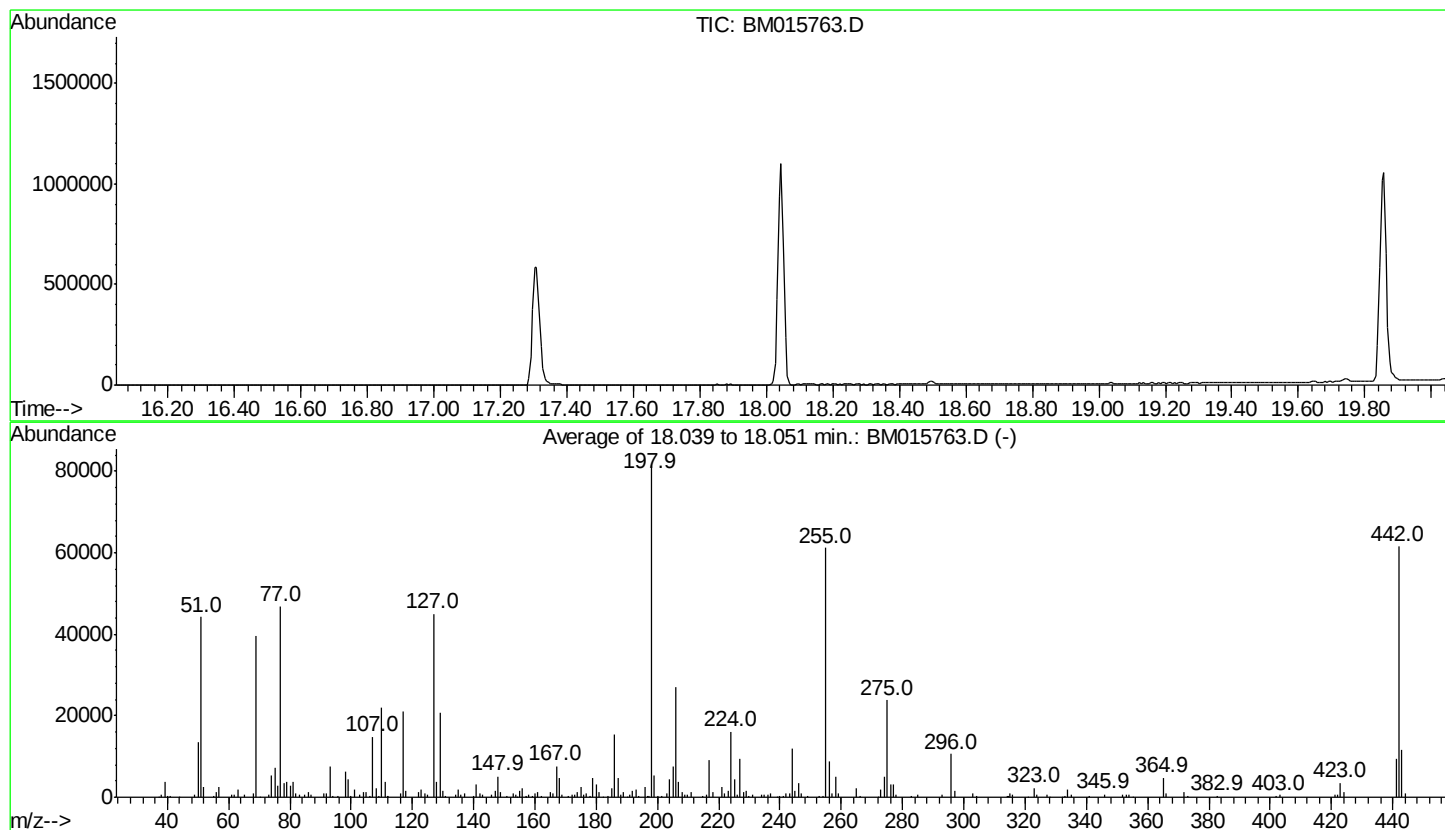

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	44194	PASS
68	69	0.00	2	2.0	799	PASS
69	198	0.00	100	48.7	39629	PASS
70	69	0.00	2	0.3	100	PASS
127	198	10	80	55.3	45024	PASS
197	198	0.00	2	0.5	389	PASS
198	198	100	100	100.0	81410	PASS
199	198	5	9	6.6	5404	PASS
275	198	10	60	29.3	23861	PASS
365	198	1	100	6.0	4870	PASS
441	443	0.01	100	79.3	9285	PASS
442	198	50	100	75.5	61458	PASS
443	442	15	24	19.1	11709	PASS