


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070518\
 Data File : BM015783.D
 Acq On : 06 Jul 2018 03:21
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 05 17:39:50 2018

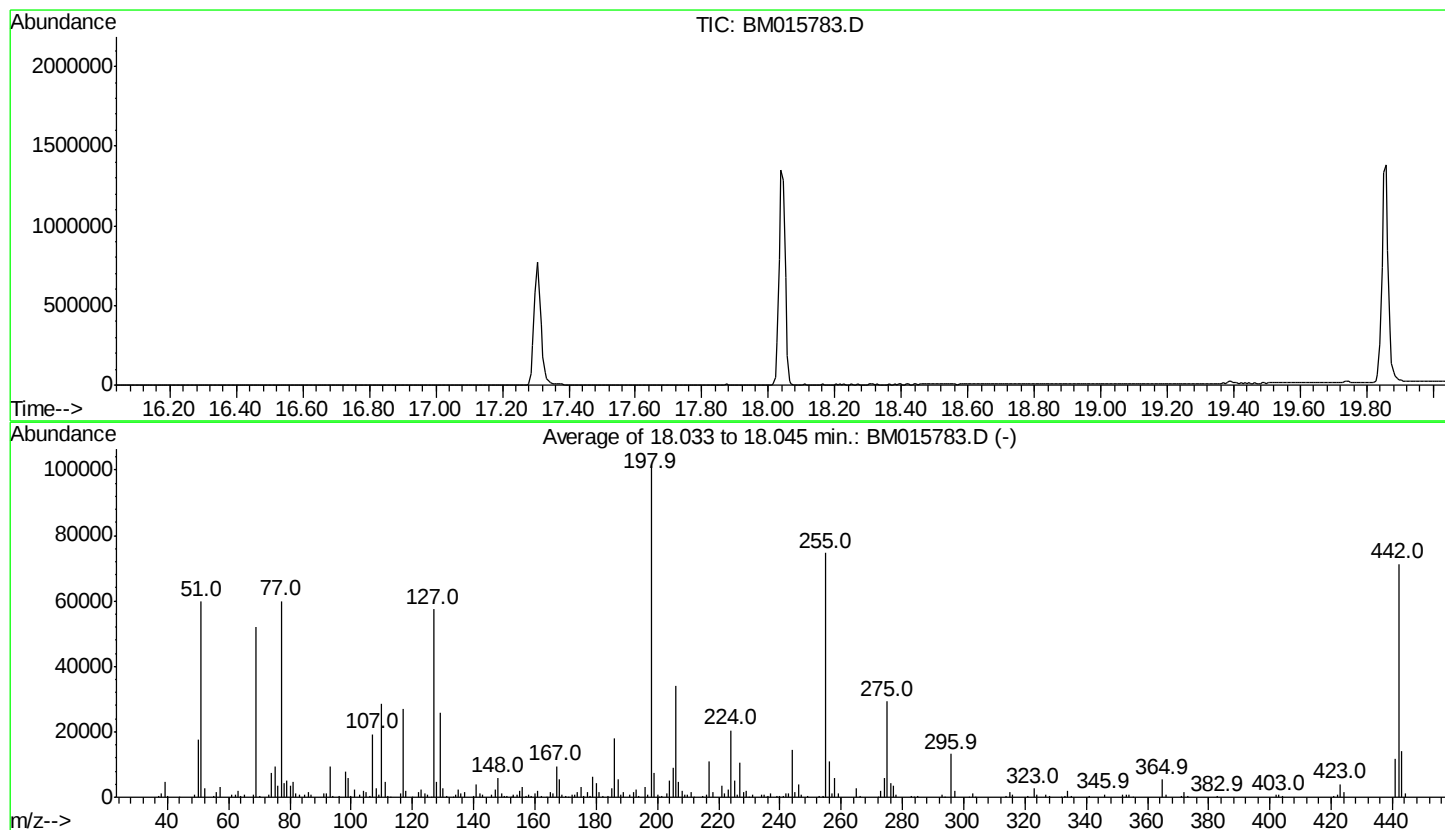

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.9	59696	PASS
68	69	0.00	2	1.9	969	PASS
69	198	0.00	100	51.3	51986	PASS
70	69	0.00	2	0.4	215	PASS
127	198	10	80	56.7	57440	PASS
197	198	0.00	2	0.7	726	PASS
198	198	100	100	100.0	101336	PASS
199	198	5	9	7.3	7421	PASS
275	198	10	60	28.8	29224	PASS
365	198	1	100	5.3	5416	PASS
441	443	0.01	100	82.1	11558	PASS
442	198	50	100	70.4	71301	PASS
443	442	15	24	19.7	14070	PASS