

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070519\
 Data File : BM021393.D
 Acq On : 05 Jul 2019 12:48
 Operator : HP/JU
 Sample : K3675-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5AF4

Quant Time: Jul 05 23:02:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 01:58:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	193186	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	903166	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.39	164	591814	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1336718	20.00	ng/ul	0.00
77) Chrysene-d12	21.32	240	977197	20.00	ng/ul	0.00
85) Perylene-d12	23.59	264	1114742	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	23839	5.86	ng/uL	0.00
5) Phenol-d5	6.92	99	545959	32.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	306659	30.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	450856	33.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	480576	34.24	ng/ul	0.00
19) Nitrobenzene-d5	8.91	128	244487	33.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	285078	35.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	557670	33.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	689822	39.95	ng/ul	0.00
43) Dimethylphthalate-d6	13.80	166	1746095	32.65	ng/ul	0.00
46) Acenaphthylene-d8	14.08	160	2058511	31.45	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	183874	21.14	ng/ul	0.00
57) Fluorene-d10	15.38	176	1543897	33.19	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	175338	21.34	ng/ul	0.00
70) Anthracene-d10	17.23	188	2261953	32.56	ng/ul	0.00
78) Pyrene-d10	19.53	212	2150513	36.67	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.44	264	2104131	31.99	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.95	94	26076	1.640	ng/ul 94
44) Dimethylphthalate	13.84	163	402343	8.265	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070519\
Data File : BM021393.D
Acq On : 05 Jul 2019 12:48
Operator : HP/JU
Sample : K3675-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5AF4

Quant Time: Jul 05 23:02:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 01:58:18 2019
Response via : Initial Calibration

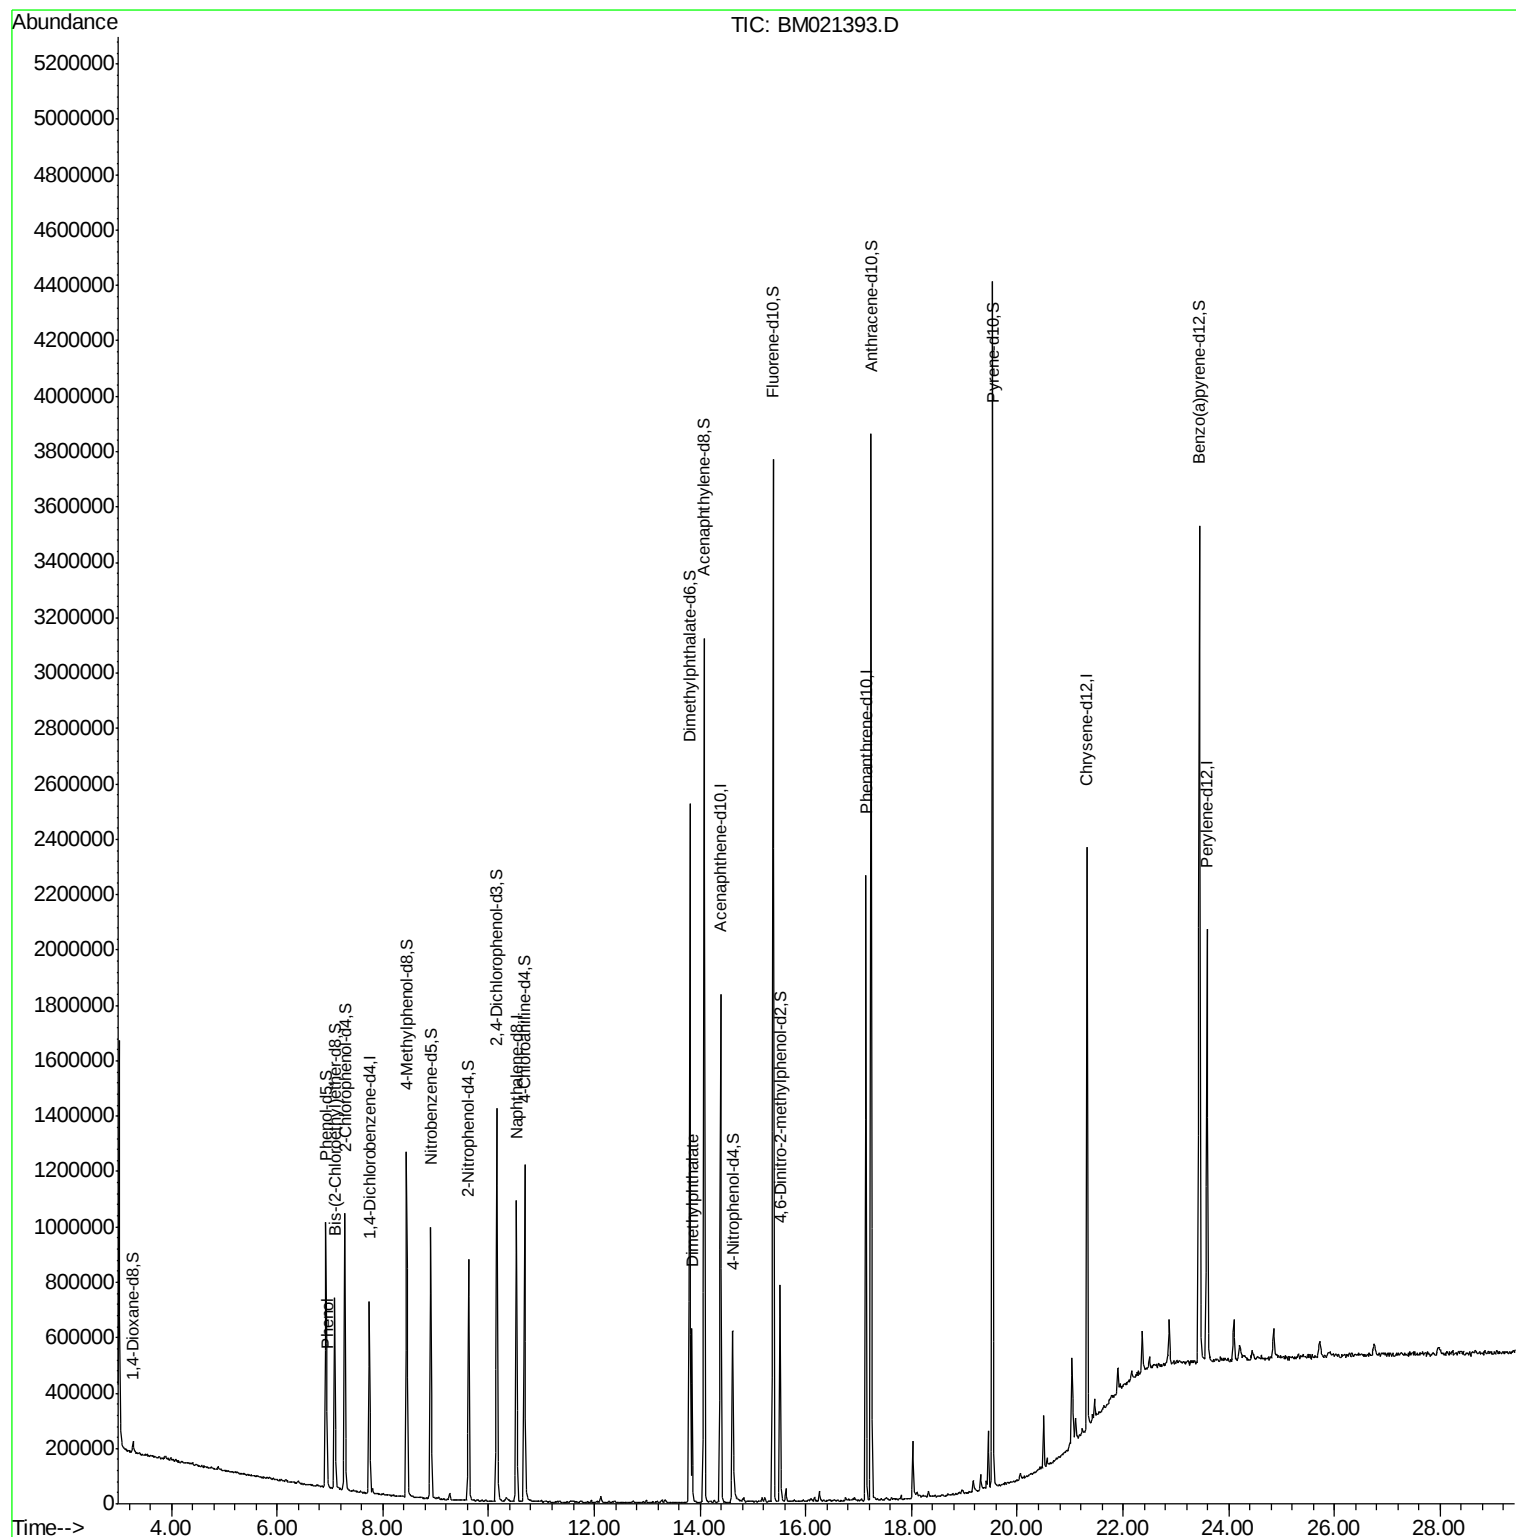

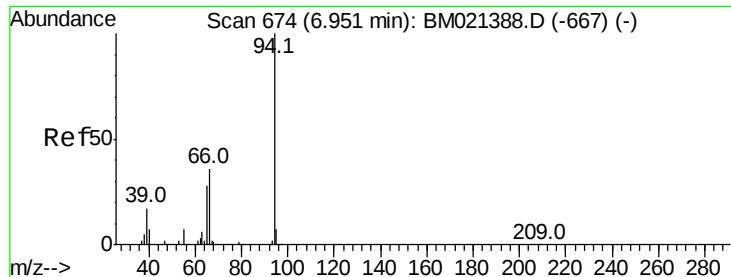

#6

Phenol

Concen: 1.640 ng/ul

RT: 6.95 min Scan# 673

Delta R.T. -0.00 min

Lab File: BM021393.D

Acq: 05 Jul 2019 12:48

Instrument :

BNA_M

ClientSampleId :

C5AF4





Tot Ion: 94 Resp: 26076

Ion Ratio Lower Upper

94 100

65 29.2 22.6 34.0

66 45.0 31.2 46.8

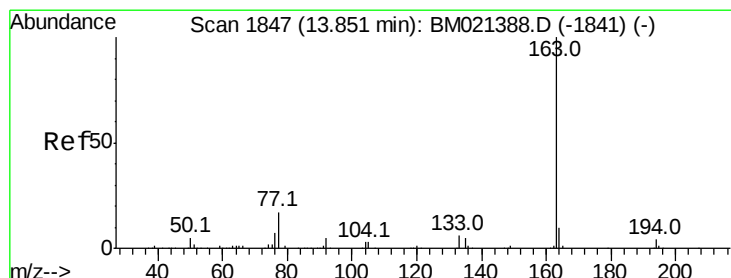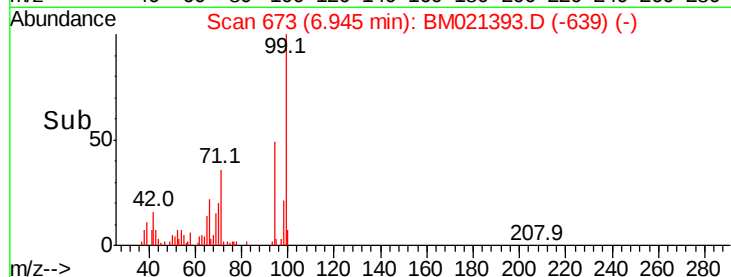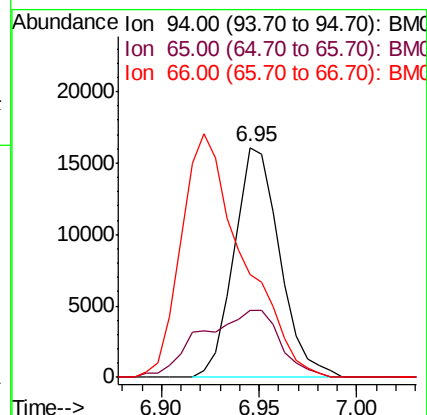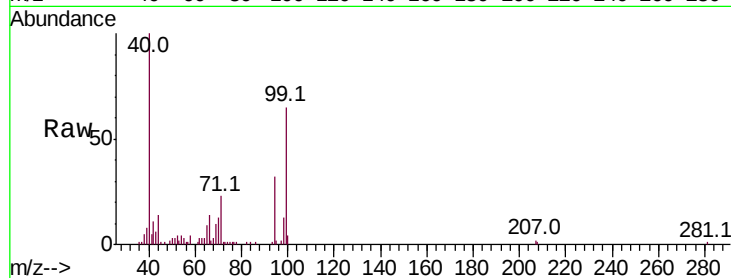

#44

Dimethylphthalate

Concen: 8.265 ng/ul

RT: 13.84 min Scan# 1846

Delta R.T. -0.01 min

Lab File: BM021393.D

Acq: 05 Jul 2019 12:48

Tgt Ion: 163 Resp: 402343

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 10.3 7.7 11.5

