

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070519\
 Data File : BM021390.D
 Acq On : 05 Jul 2019 10:59
 Operator : HP/JU
 Sample : PB121157BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	46	48	55	rVB2	38429	56864	1.14%	0.106%
2	6.922	663	669	682	rVB	901449	1416661	28.36%	2.630%
3	7.087	691	697	710	rVB	657185	1051285	21.04%	1.952%
4	7.281	723	730	740	rVB	934155	1480148	29.63%	2.748%
5	7.745	802	809	818	rVB	601024	976162	19.54%	1.812%
6	8.451	923	929	940	rBV	1155591	1918768	38.41%	3.562%
7	8.910	999	1007	1022	rVB	916760	1559548	31.22%	2.895%
8	9.622	1121	1128	1143	rBV	827030	1339384	26.81%	2.487%
9	10.157	1212	1219	1235	rBV	1310057	2230984	44.66%	4.142%
10	10.528	1275	1282	1291	rVB	962154	1586382	31.75%	2.945%
11	10.681	1300	1308	1326	rBV	1201932	2159635	43.23%	4.009%
12	12.122	1545	1553	1562	rBV	18643	33275	0.67%	0.062%
13	13.804	1832	1839	1849	rBV	2366409	3294082	65.94%	6.115%
14	14.080	1879	1886	1900	rBV	2873928	4138131	82.83%	7.682%
15	14.386	1931	1938	1948	rBV2	1538686	2332185	46.68%	4.330%
16	14.616	1969	1977	1998	rBV	484405	965721	19.33%	1.793%
17	15.380	2100	2107	2118	rBV	3544770	4995724	100.00%	9.274%
18	15.516	2124	2130	2143	rBV	565818	807573	16.17%	1.499%
19	15.621	2143	2148	2153	rVB2	37733	50431	1.01%	0.094%
20	16.168	2237	2241	2247	rVB2	11209	14641	0.29%	0.027%
21	16.927	2365	2370	2374	rVB2	5752	8953	0.18%	0.017%
22	17.139	2399	2406	2416	rBV2	1730045	2507833	50.20%	4.656%
23	17.233	2416	2422	2437	rBV	3216953	4678589	93.65%	8.686%
24	19.168	2745	2751	2758	rBV	29546	55757	1.12%	0.104%
25	19.421	2790	2794	2798	rBV	20937	26838	0.54%	0.050%
26	19.533	2807	2813	2824	rBV	3528527	4731613	94.71%	8.784%
27	21.321	3112	3117	3125	rBV	1756637	2285308	45.75%	4.243%
28	23.444	3471	3478	3490	rVB	2619922	4750620	95.09%	8.819%
29	23.586	3496	3502	3514	rVB	1258428	2412768	48.30%	4.479%


Sum of corrected areas: 53865863

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070519\
Data File : BM021390.D
Acq On : 05 Jul 2019 10:59
Operator : HP/JU
Sample : PB121157BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

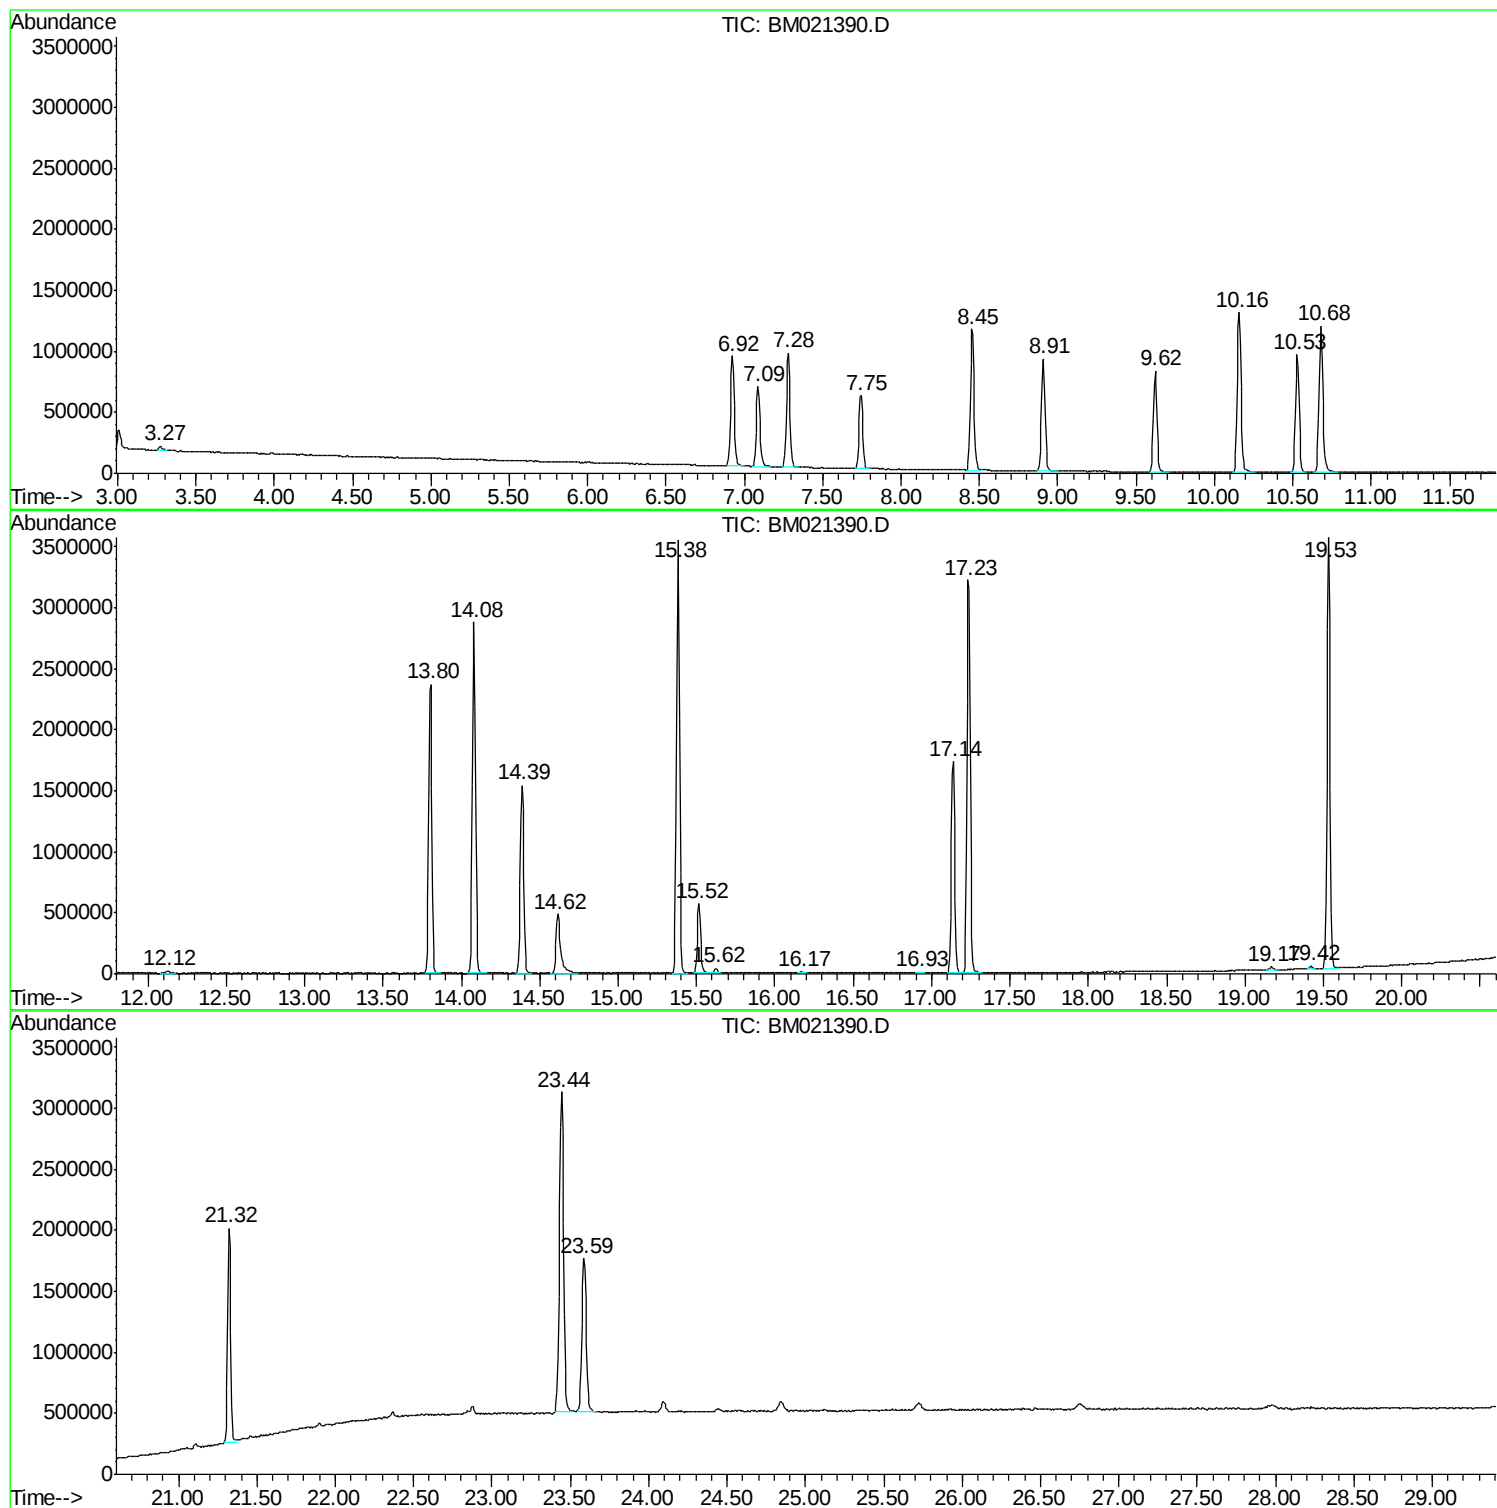

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070519\
Data File : BM021390.D
Acq On : 05 Jul 2019 10:59
Operator : HP/JU
Sample : PB121157BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070519\
Data File : BM021390.D
Acq On : 05 Jul 2019 10:59
Operator : HP/JU
Sample : PB121157BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc