

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040724.D
 Acq On : 07 Jul 2023 22:04
 Operator : MA/JU
 Sample : PB153638BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK638

Quant Time: Jul 08 05:11:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 10:22:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.895	152	4358	0.400	ng/ul	0.00
4) Naphthalene-d8	10.702	136	16427	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.541	164	9088	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.291	188	17363	0.400	ng/ul	0.00
17) Chrysene-d12	21.483	240	10182	0.400	ng/ul	0.00
23) Perylene-d12	23.877	264	11326	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	34065	4.976	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	7004	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.324	212	11215	0.344	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.687	202	2843	0.061	ng/ul#	1
26) Benzo(a)pyrene	23.725	252	4399	0.111	ng/ul#	21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040724.D
Acq On : 07 Jul 2023 22:04
Operator : MA/JU
Sample : PB153638BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK638

Quant Time: Jul 08 05:11:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 10:22:24 2023
Response via : Initial Calibration




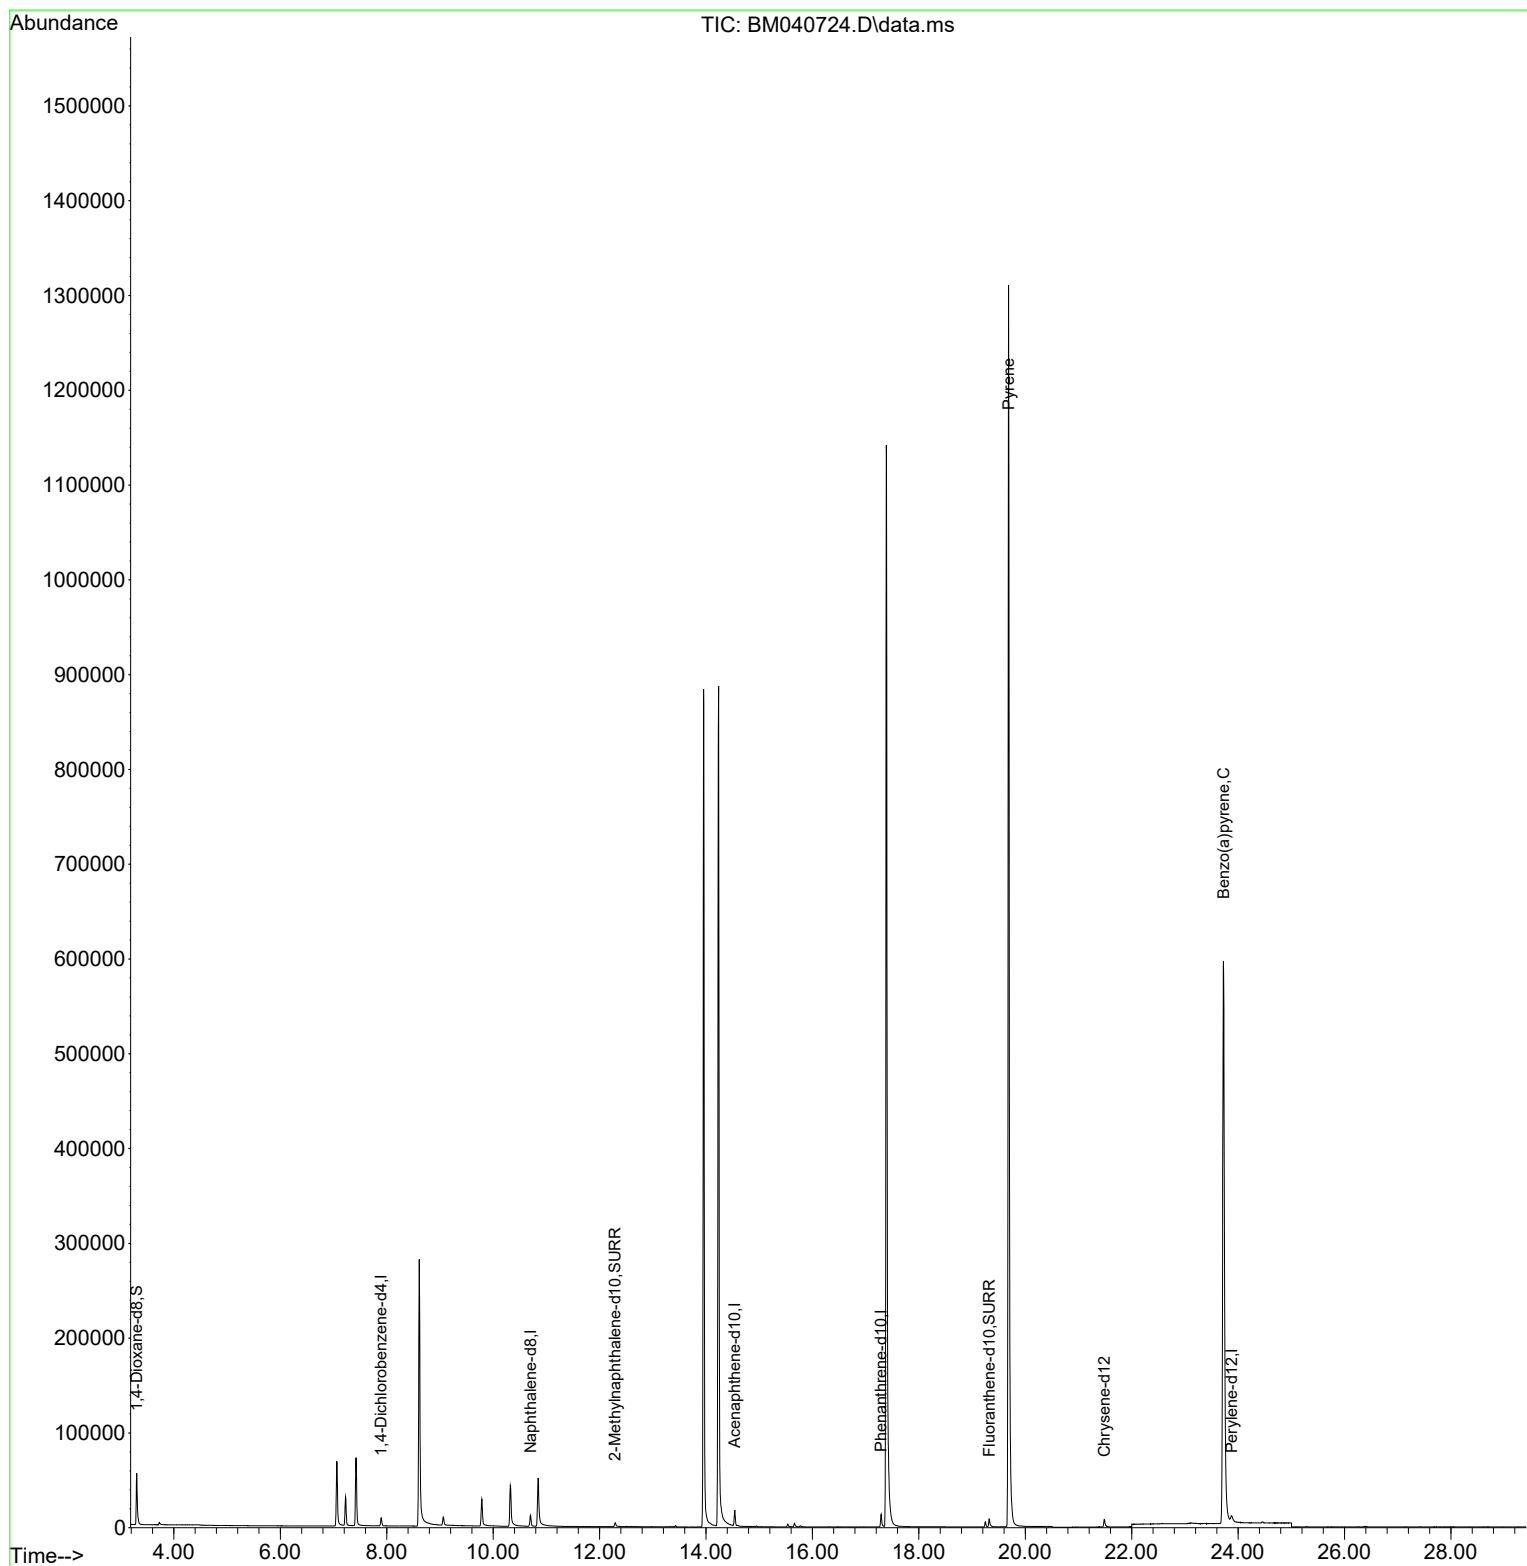


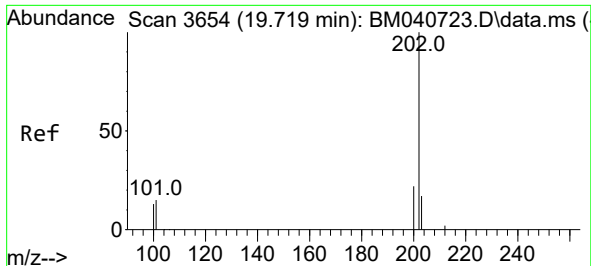

#20
Pyrene
Concen: 0.061 ng/ul
RT: 19.687 min Scan# 3647
Delta R.T. -0.033 min
Lab File: BM040724.D
Acq: 07 Jul 2023 22:04

Instrument :
BNA_M
ClientSampleId :
SBLK638

Tgt Ion:202 Resp: 2843
Ion Ratio Lower Upper
202 100
101 191.6 12.6 18.8#
100 1420.9 9.8 14.6#

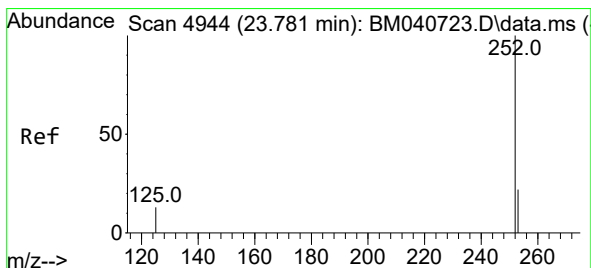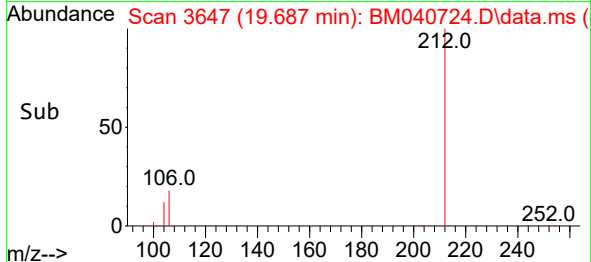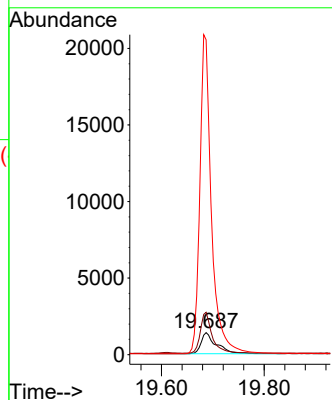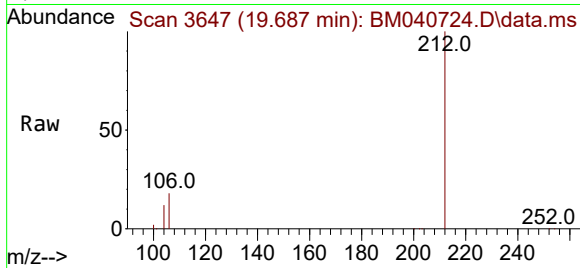

#26
Benzo(a)pyrene
Concen: 0.111 ng/ul
RT: 23.725 min Scan# 4925
Delta R.T. -0.053 min
Lab File: BM040724.D
Acq: 07 Jul 2023 22:04

Tgt Ion:252 Resp: 4399
Ion Ratio Lower Upper
252 100
253 59.7 22.9 34.3#
125 78.5 21.0 31.4#

