

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040725.D
 Acq On : 07 Jul 2023 22:42
 Operator : MA/JU
 Sample : 03237-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBW81

Quant Time: Jul 08 05:11:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 10:22:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	4961	0.400	ng/ul	0.00
4) Naphthalene-d8	10.702	136	19004	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.541	164	11263	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.291	188	19370	0.400	ng/ul	0.00
17) Chrysene-d12	21.483	240	11399	0.400	ng/ul	0.00
23) Perylene-d12	23.874	264	12566	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	23139	2.969	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.297	152	6889	0.259	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	12513	0.342	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.536	166	3154	0.070	ng/ul#	19
20) Pyrene	19.687	202	2607	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.722	252	4296	0.098	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040725.D
Acq On : 07 Jul 2023 22:42
Operator : MA/JU
Sample : 03237-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBW81

Quant Time: Jul 08 05:11:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 10:22:24 2023
Response via : Initial Calibration




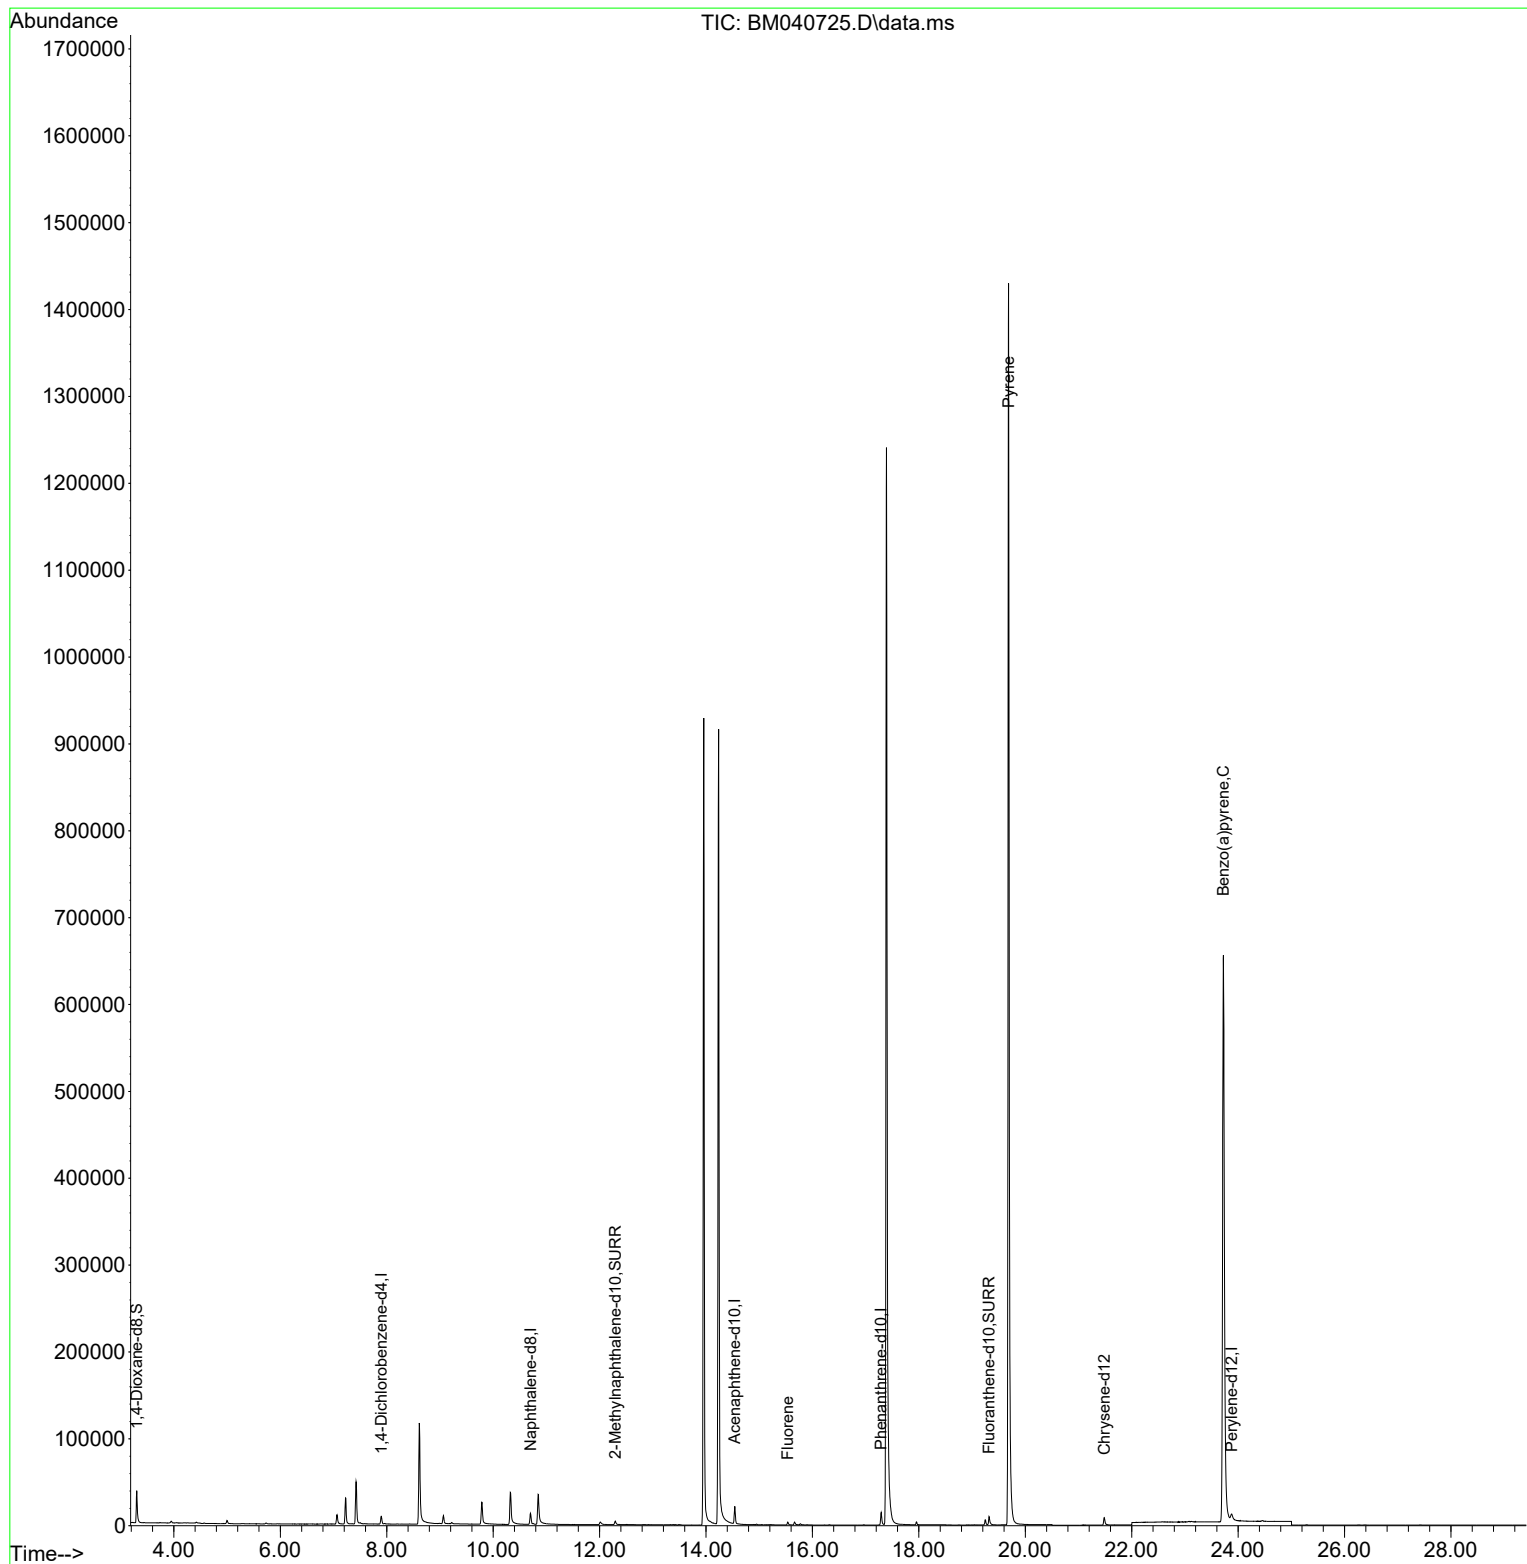


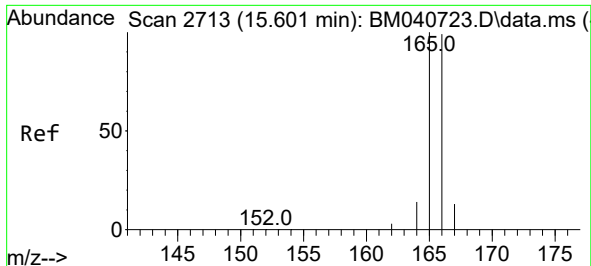

#12
Fluorene
Concen: 0.070 ng/ul
RT: 15.536 min Scan# 21
Delta R.T. -0.065 min
Lab File: BM040725.D
Acq: 07 Jul 2023 22:42




Instrument :
BNA_M
ClientSampleId :
YBW81


Tgt Ion:166 Resp: 3154
Ion Ratio Lower Upper
166 100
165 14.2 79.6 119.4#
167 33.0 11.4 17.0#

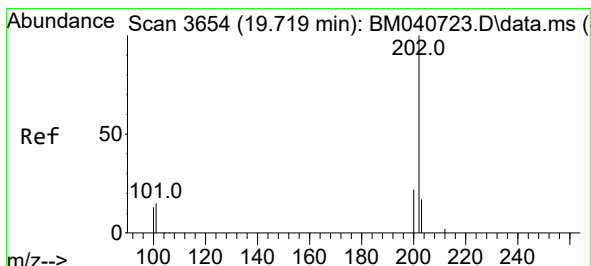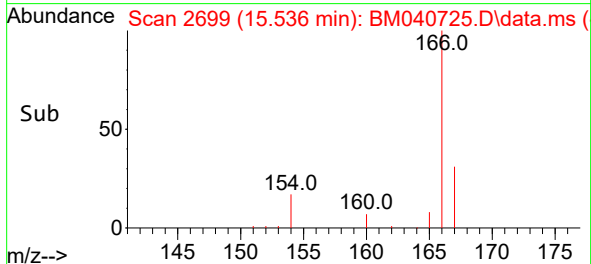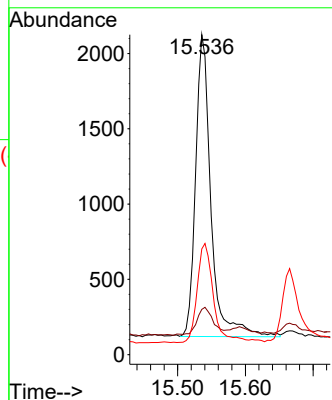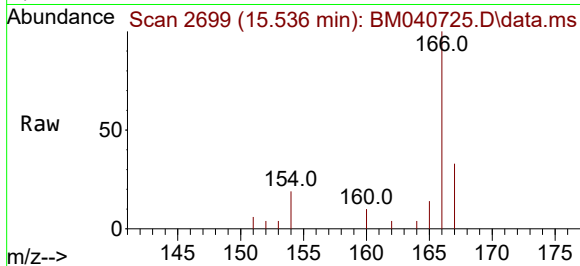

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.687 min Scan# 3647
Delta R.T. -0.033 min
Lab File: BM040725.D
Acq: 07 Jul 2023 22:42


Tgt Ion:202 Resp: 2607
Ion Ratio Lower Upper
202 100
101 177.4 12.6 18.8#
100 1301.7 9.8 14.6#

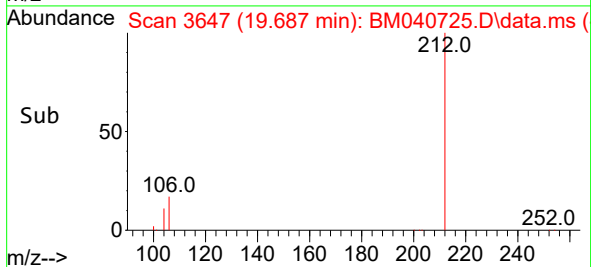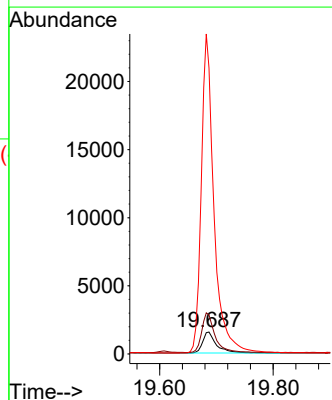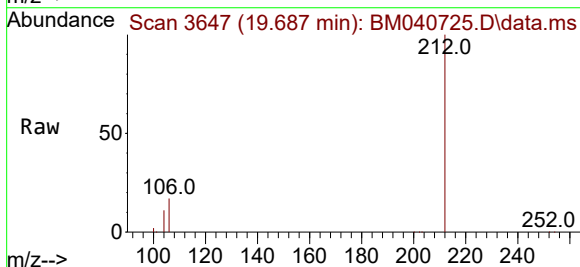

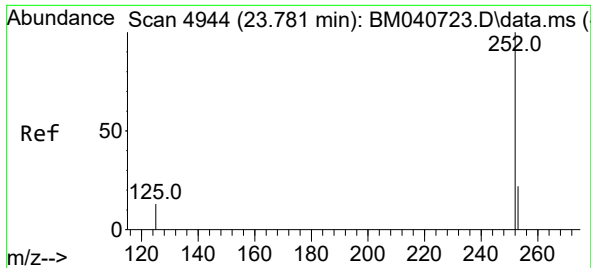

#26
Benzo(a)pyrene
Concen: 0.098 ng/ul
RT: 23.722 min Scan# 4944
Delta R.T. -0.056 min
Lab File: BM040725.D
Acq: 07 Jul 2023 22:42

Instrument :
BNA_M
ClientSampleId :
YBW81

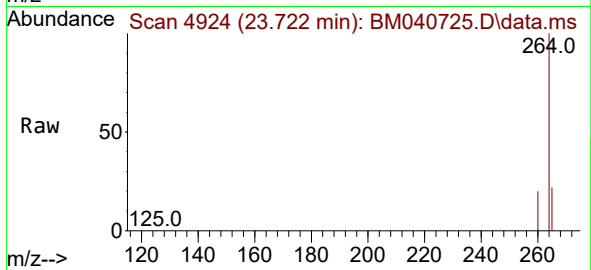

Tgt Ion:252 Resp: 4296
Ion Ratio Lower Upper
252 100
253 57.3 22.9 34.3#
125 68.1 21.0 31.4#

