




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040671.D
 Acq On : 06 Jul 2023 11:19
 Operator : MA/JU
 Sample : 03248-06DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCGN4DL

Manual IntegrationsAPPROVED

Quant Time: Jul 06 11:50:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 09:30:35 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/06/2023
 Supervised By :Sohil Jodhani 07/06/2023

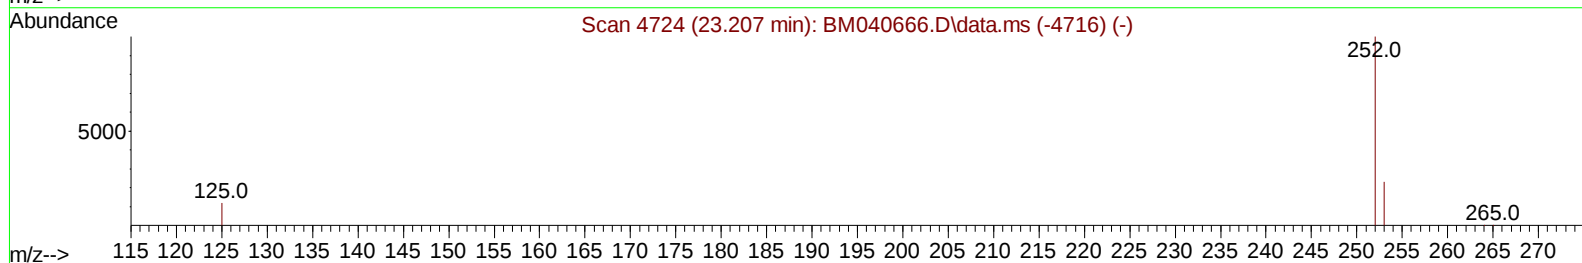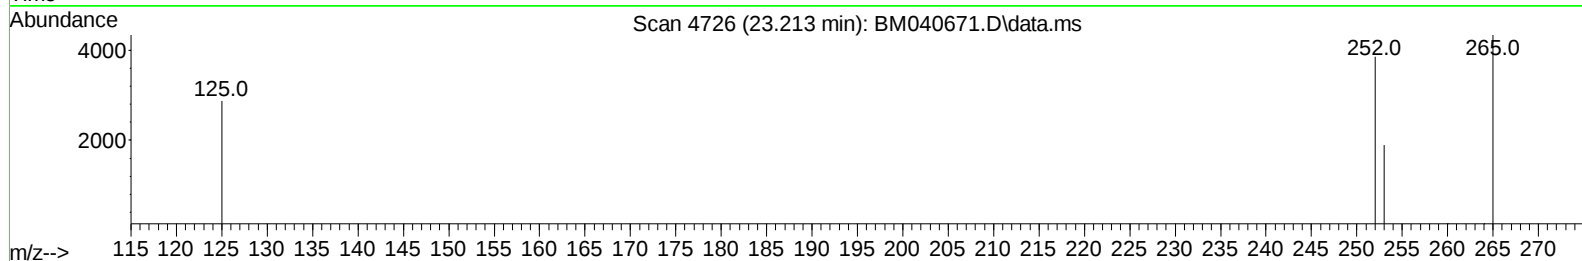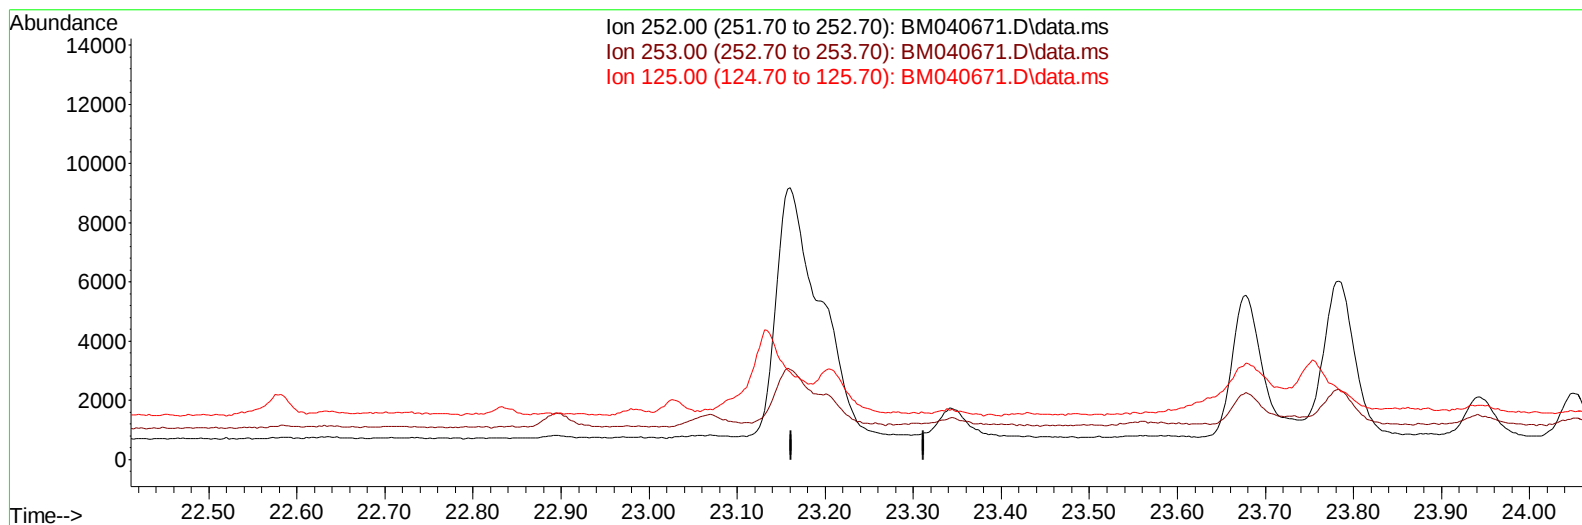

TIC: BM040671.D\data.ms

(25) Benzo(k)fluoranthene

23.212min (-23.212) 0.00 ng/u1

response 0

Ion	Exp%	Act%
252.00	100.00	0.00
253.00	26.50	0.00#
125.00	20.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040671.D
Acq On : 06 Jul 2023 11:19
Operator : MA/JU
Sample : 03248-06DL 5X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCGN4DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/06/2023
Supervised By :Sohil Jodhani 07/06/2023

Quant Time: Jul 06 11:50:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 09:30:35 2023
Response via : Initial Calibration

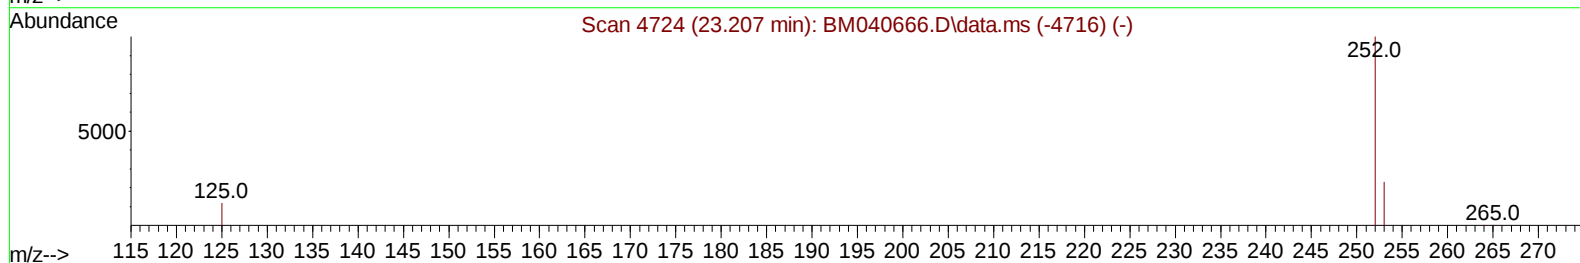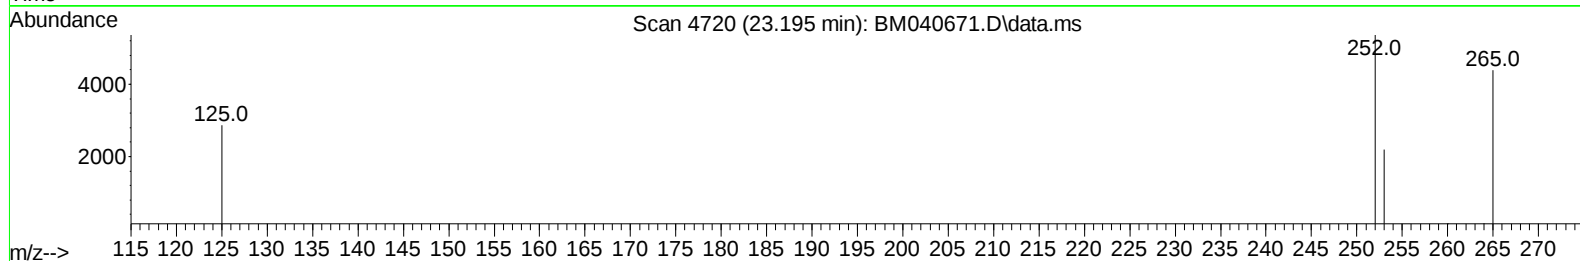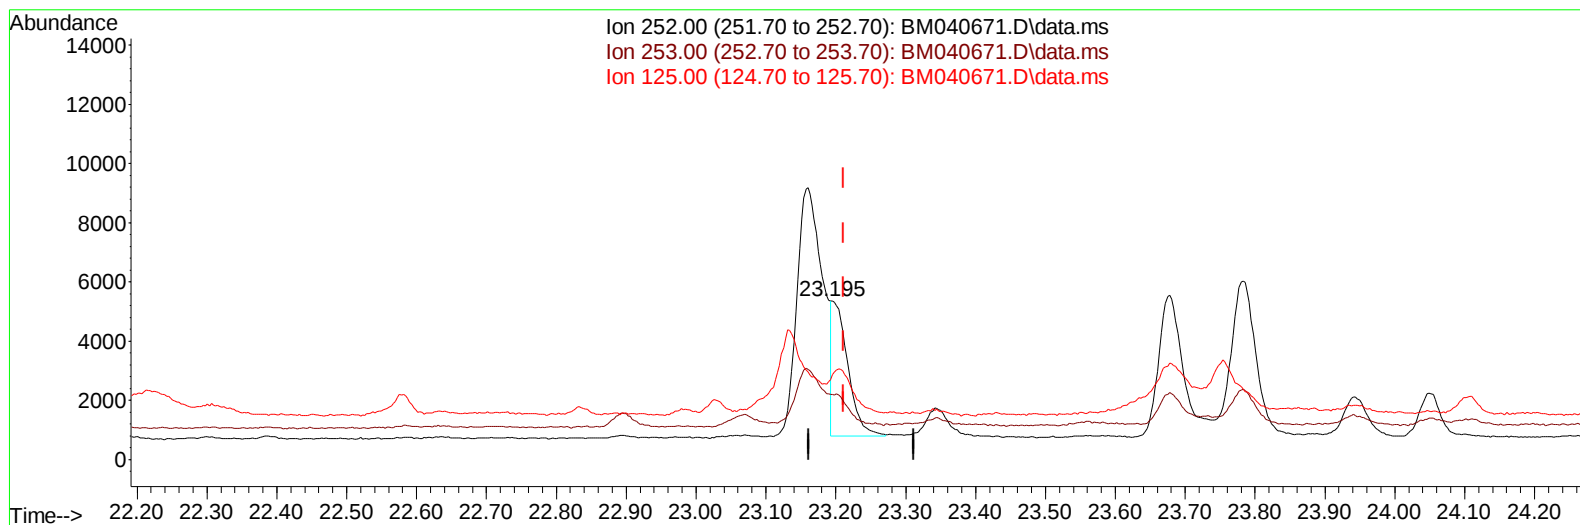

TIC: BM040671.D\data.ms

(25) Benzo(k)fluoranthene

23.195min (-0.016) 0.06 ng/u1 m

response 7218

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	41.04#
125.00	20.50	53.42#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040671.D
 Acq On : 06 Jul 2023 11:19
 Operator : MA/JU
 Sample : 03248-06DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCGN4DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/06/2023
 Supervised By :Sohil Jodhani 07/06/2023

Quant Time: Jul 06 11:50:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 09:30:35 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.907	152		13310	0.400	ng/ul	0.00
4) Naphthalene-d8	10.712	136		48940	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.549	164		23260	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.303	188		42627	0.400	ng/ul	0.00
17) Chrysene-d12	21.488	240		27861	0.400	ng/ul	0.00
23) Perylene-d12	23.891	264		30018	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.312	96		9230	0.441	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.307	152		2368	0.035	ng/ul	0.00
18) Fluoranthene-d10	19.328	212		3307	0.037	ng/ul	0.00
Target Compounds							
						Qvalue	
15) Phenanthrene	17.341	178		7554	0.057	ng/ul#	90
19) Fluoranthene	19.361	202		19840	0.168	ng/ul	99
20) Pyrene	19.723	202		17939	0.141	ng/ul#	94
21) Benzo(a)anthracene	21.471	228		10516	0.112	ng/ul#	92
22) Chrysene	21.523	228		11038	0.103	ng/ul#	94
24) Benzo(b)fluoranthene	23.160	252		23010	0.198	ng/ul	83
25) Benzo(k)fluoranthene	23.195	252		7218m	0.063	ng/ul	
26) Benzo(a)pyrene	23.783	252		12645	0.121	ng/ul#	77
27) Indeno(1,2,3-cd)pyrene	26.373	276		12572	0.086	ng/ul#	88
28) Dibenzo(a,h)anthracene	26.390	278		3081	0.027	ng/ul#	30
29) Benzo(g,h,i)perylene	27.145	276		10726	0.084	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040671.D
Acq On : 06 Jul 2023 11:19
Operator : MA/JU
Sample : 03248-06DL 5X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCGN4DL

Manual IntegrationsAPPROVED

Quant Time: Jul 06 11:50:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 09:30:35 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/06/2023
Supervised By :Sohil Jodhani 07/06/2023

