

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040652.D
 Acq On : 05 Jul 2023 22:49
 Operator : MA/JU
 Sample : 03257-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXYT9

Quant Time: Jul 06 00:38:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 09:30:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	6312	0.400	ng/u1	0.00
4) Naphthalene-d8	10.718	136	22761	0.400	ng/u1 #	0.00
9) Acenaphthene-d10	14.554	164	11538	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.303	188	19504	0.400	ng/u1	0.00
17) Chrysene-d12	21.491	240	10759	0.400	ng/u1	0.00
23) Perylene-d12	23.891	264	13609	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.312	96	35002	3.530	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.307	152	8477	0.266	ng/u1	0.00
18) Fluoranthene-d10	19.333	212	13472	0.391	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.346	88	9879	0.979	ng/u1	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040652.D
Acq On : 05 Jul 2023 22:49
Operator : MA/JU
Sample : 03257-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXYT9

Quant Time: Jul 06 00:38:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 09:30:35 2023
Response via : Initial Calibration

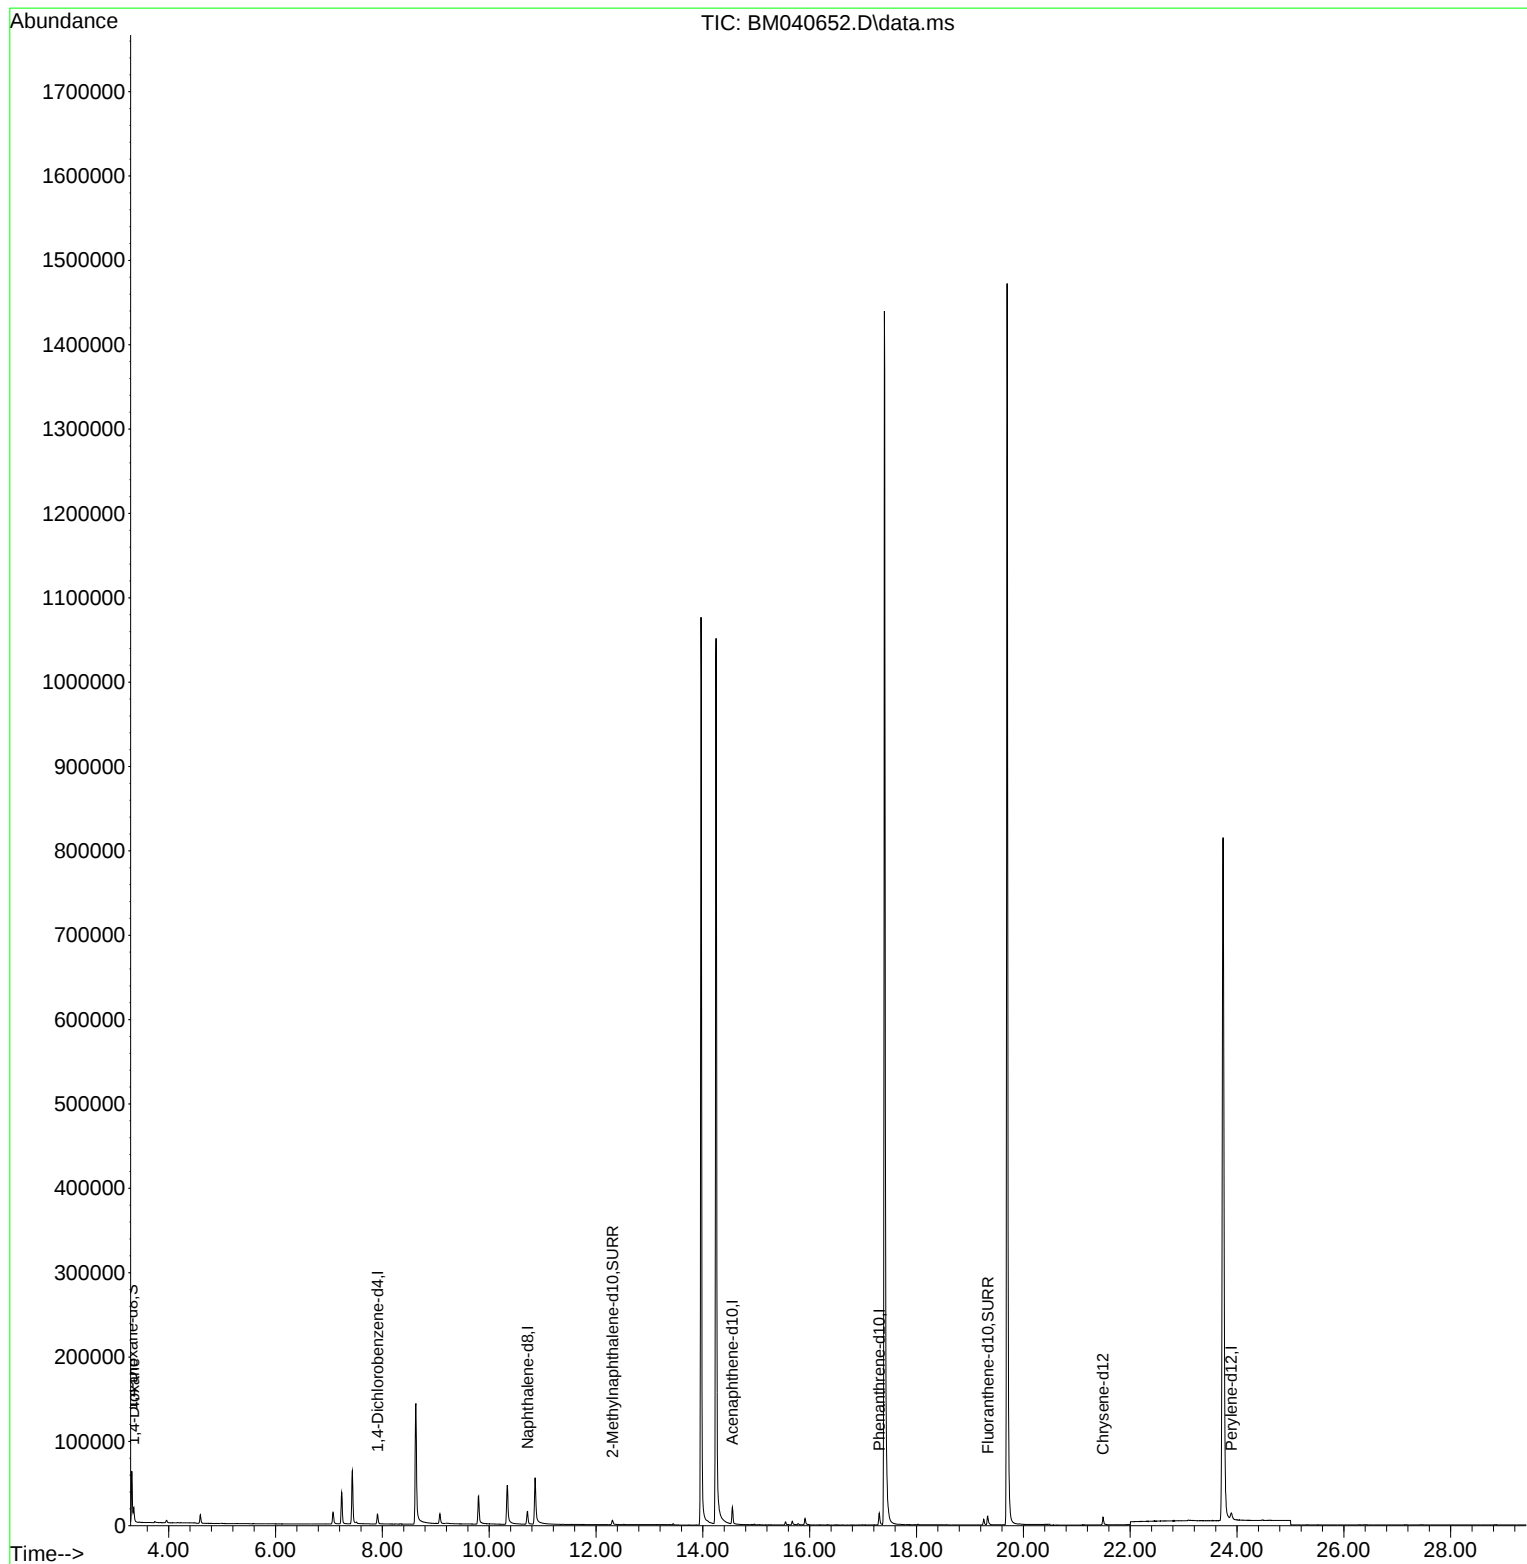

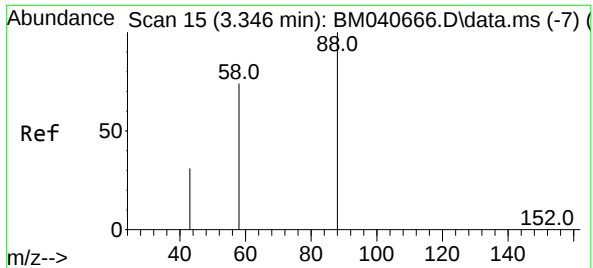

1,4-Dioxane
 Concen: 0.979 ng/ul
 RT: 3.346 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BM040652.D
 Acq: 05 Jul 2023 22:49

Instrument :
 BNA_M
 ClientSampleId :
 EXYT9

Tgt Ion: 88 Resp: 9879

Ion	Ratio	Lower	Upper
88	100		
43	44.1	36.1	54.1
58	70.5	49.8	74.8

