

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040655.D
 Acq On : 06 Jul 2023 00:43
 Operator : MA/JU
 Sample : 03257-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXYW1

Quant Time: Jul 06 01:48:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 09:30:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.907	152	5742	0.400	ng/ul	0.00
4) Naphthalene-d8	10.712	136	21081	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.554	164	10612	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.303	188	18132	0.400	ng/ul	0.00
17) Chrysene-d12	21.488	240	9824	0.400	ng/ul	0.00
23) Perylene-d12	23.888	264	12769	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.308	96	37640	4.173	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.307	152	9512	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.328	212	15314	0.486	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.346	88	19684	2.144	ng/ul	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040655.D
Acq On : 06 Jul 2023 00:43
Operator : MA/JU
Sample : 03257-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXYW1

Quant Time: Jul 06 01:48:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 09:30:35 2023
Response via : Initial Calibration

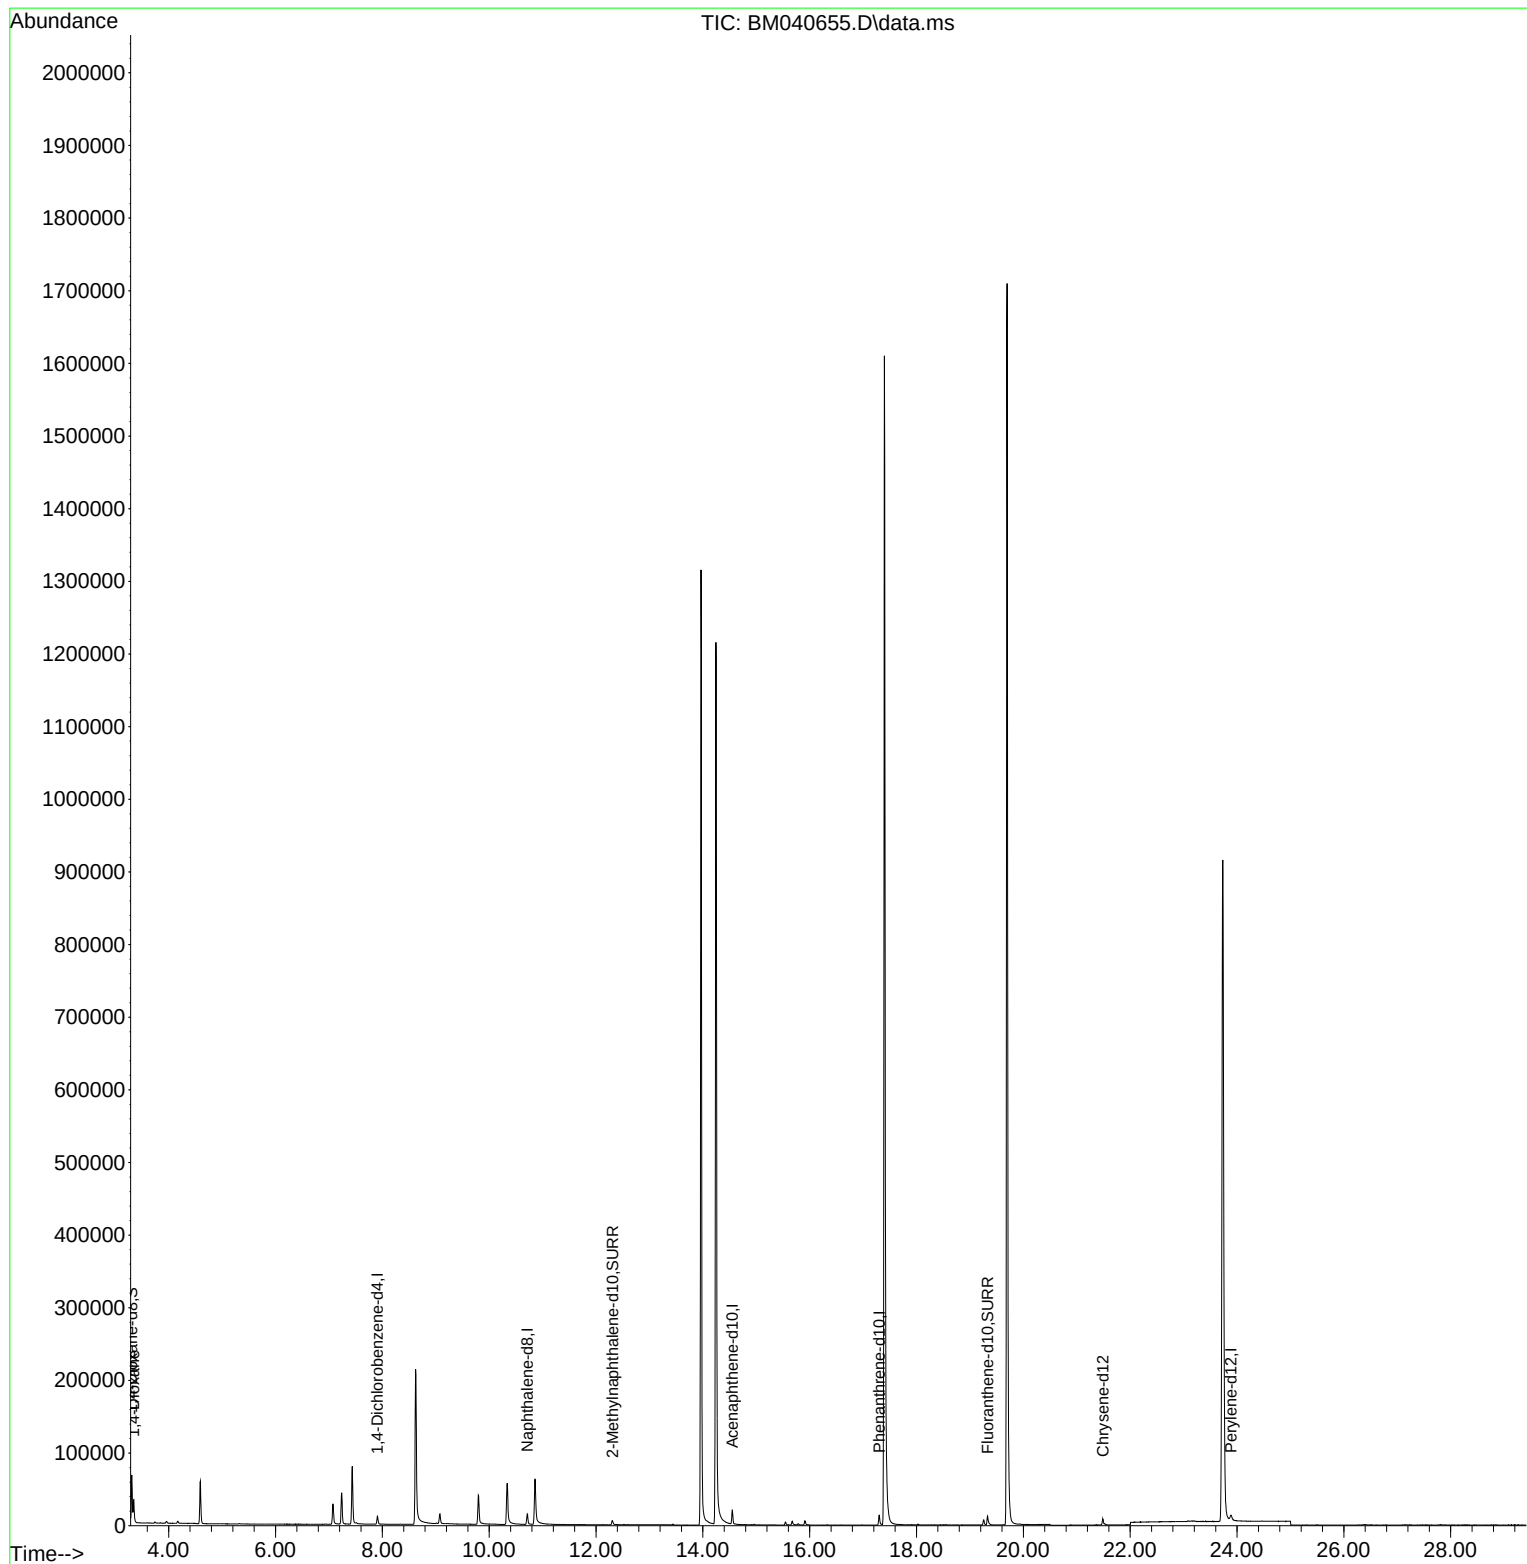

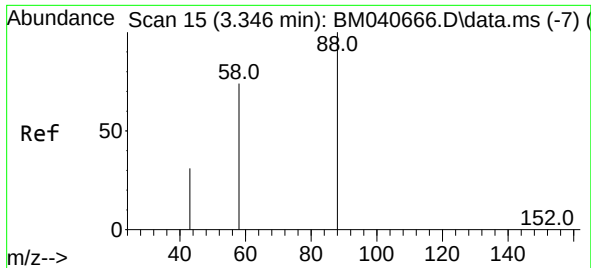

1,4-Dioxane

Concen: 2.144 ng/ul

RT: 3.346 min Scan# 11

Delta R.T. 0.000 min

Lab File: BM040655.D


Acq: 06 Jul 2023 00:43

Instrument :

BNA_M

ClientSampleId :

EXYW1

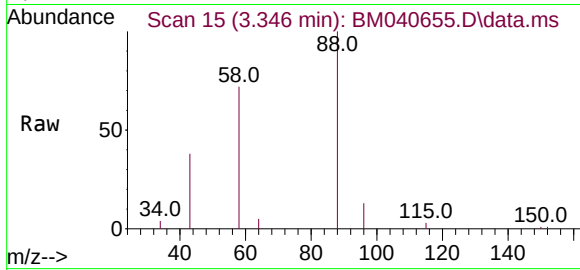

Tgt Ion: 88 Resp: 19684

Ion Ratio Lower Upper

88 100

43 38.3 36.1 54.1

58 72.4 49.8 74.8

