

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040694.D
 Acq On : 07 Jul 2023 01:58
 Operator : MA/JU
 Sample : 03257-17
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXYW3

Quant Time: Jul 07 04:28:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 09:30:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	6582	0.400	ng/u1	0.00
4) Naphthalene-d8	10.708	136	24506	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.546	164	12906	0.400	ng/u1	#-0.01
13) Phenanthrene-d10	17.295	188	22058	0.400	ng/u1	-0.01
17) Chrysene-d12	21.483	240	12253	0.400	ng/u1	-0.01
23) Perylene-d12	23.877	264	14784	0.400	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	30995	2.998	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.297	152	7934	0.231	ng/u1	-0.01
18) Fluoranthene-d10	19.325	212	12351	0.314	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.343	88	34328	3.262	ng/u1	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040694.D
Acq On : 07 Jul 2023 01:58
Operator : MA/JU
Sample : 03257-17
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXYW3

Quant Time: Jul 07 04:28:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 09:30:35 2023
Response via : Initial Calibration

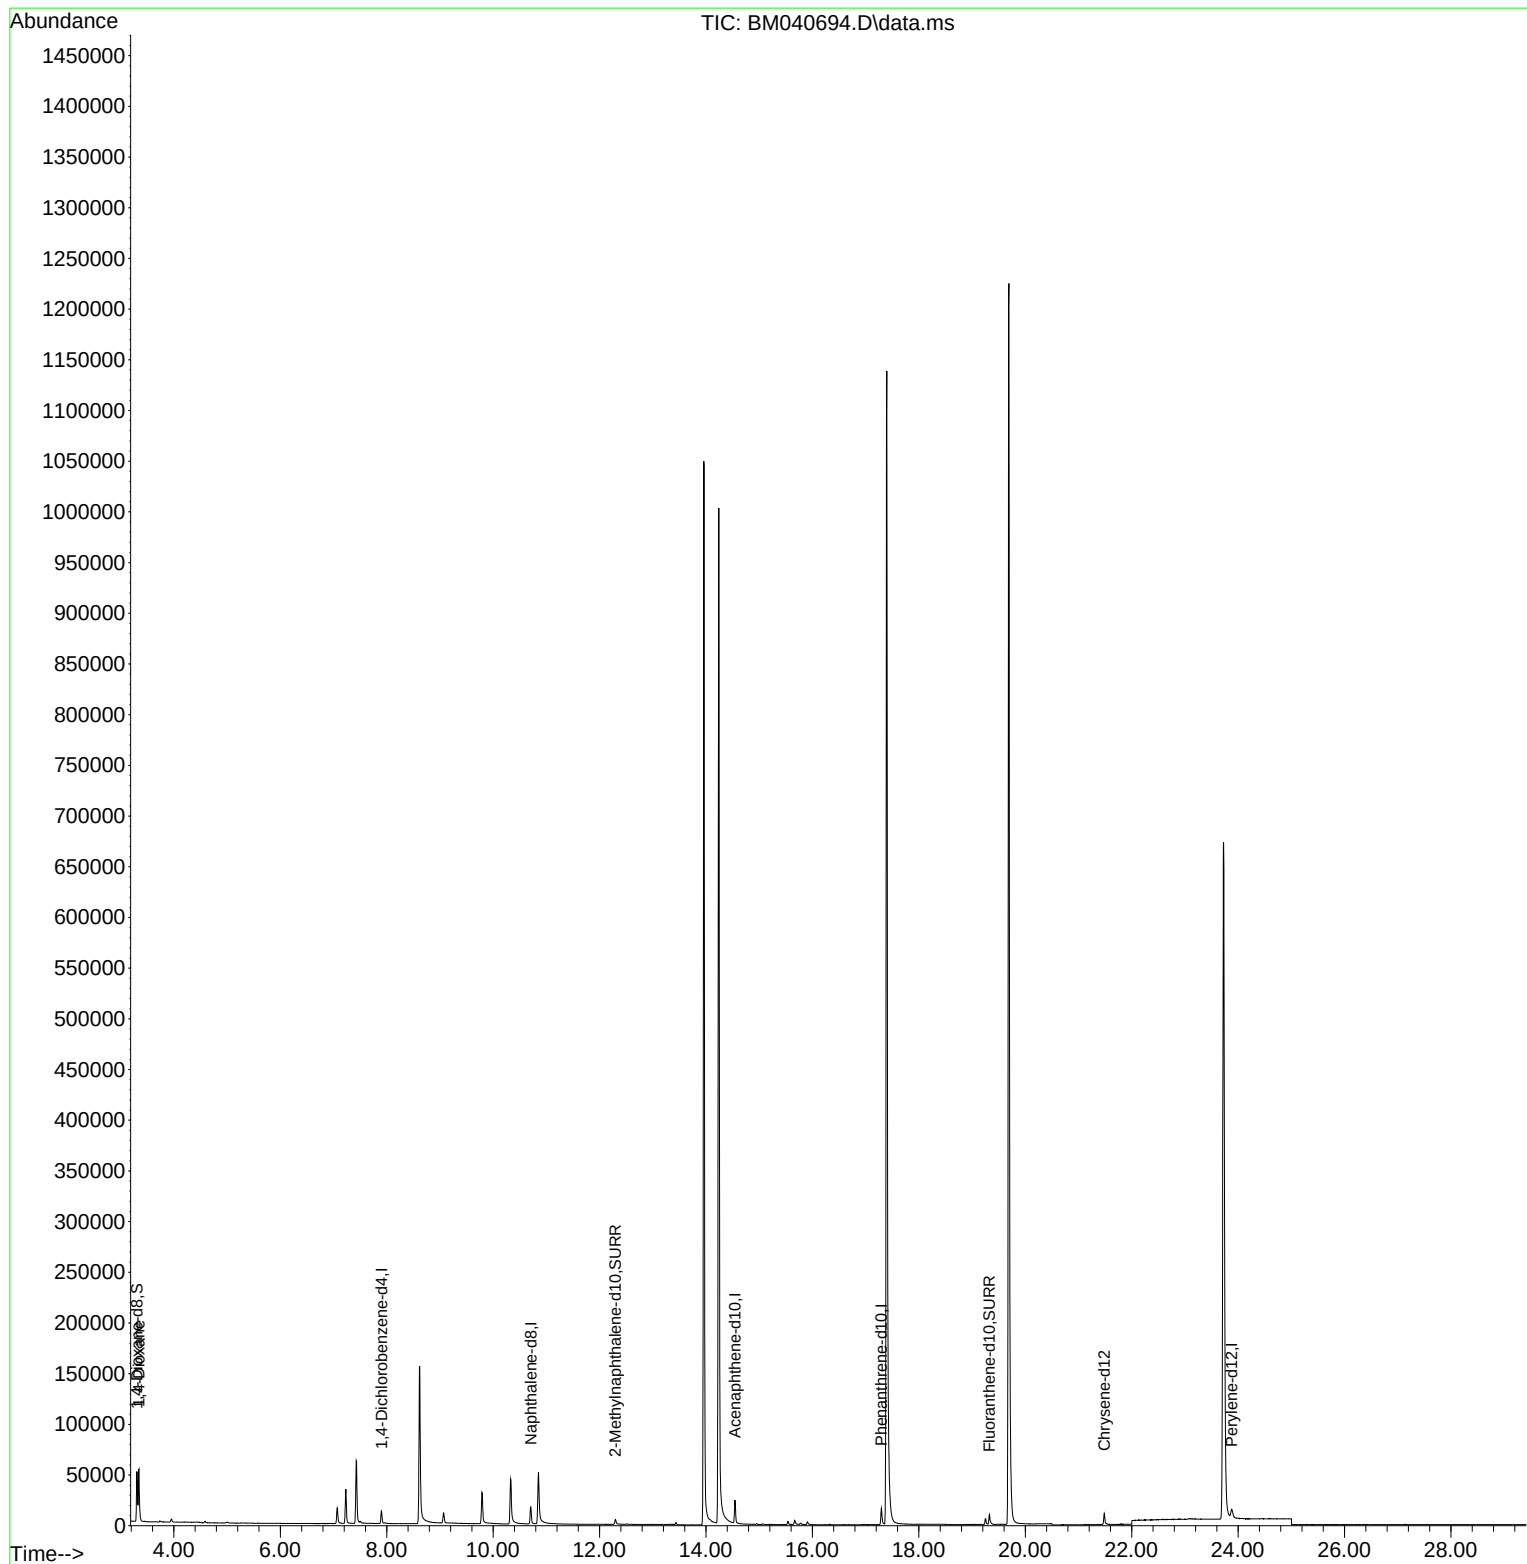

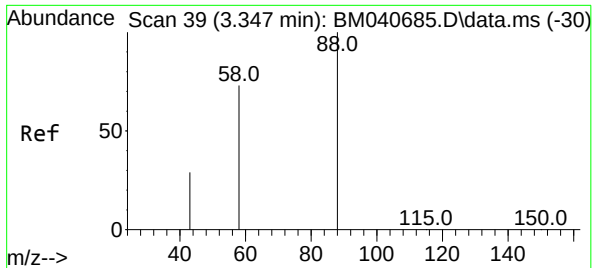

#2
 1,4-Dioxane
 Concen: 3.262 ng/ul
 RT: 3.343 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: BM040694.D
 Acq: 07 Jul 2023 01:58

Instrument :
 BNA_M
 ClientSampleId :
 EXYW3

Tgt Ion: 88 Resp: 34328
 Ion Ratio Lower Upper
 88 100
 43 36.5 36.1 54.1
 58 72.7 49.8 74.8

