

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040697.D
 Acq On : 07 Jul 2023 03:51
 Operator : MA/JU
 Sample : 03258-03
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCGW2

Quant Time: Jul 07 04:31:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 09:30:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	5943	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.708	136	21470	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.546	164	11112	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.295	188	19878	0.400	ng/ul	-0.01
17) Chrysene-d12	21.483	240	11990	0.400	ng/ul	-0.01
23) Perylene-d12	23.880	264	14250	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	32092	3.438	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.297	152	8280	0.275	ng/ul	-0.01
18) Fluoranthene-d10	19.325	212	15078	0.392	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.343	88	379	0.040	ng/ul#	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040697.D
Acq On : 07 Jul 2023 03:51
Operator : MA/JU
Sample : 03258-03
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCGW2

Quant Time: Jul 07 04:31:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 09:30:35 2023
Response via : Initial Calibration

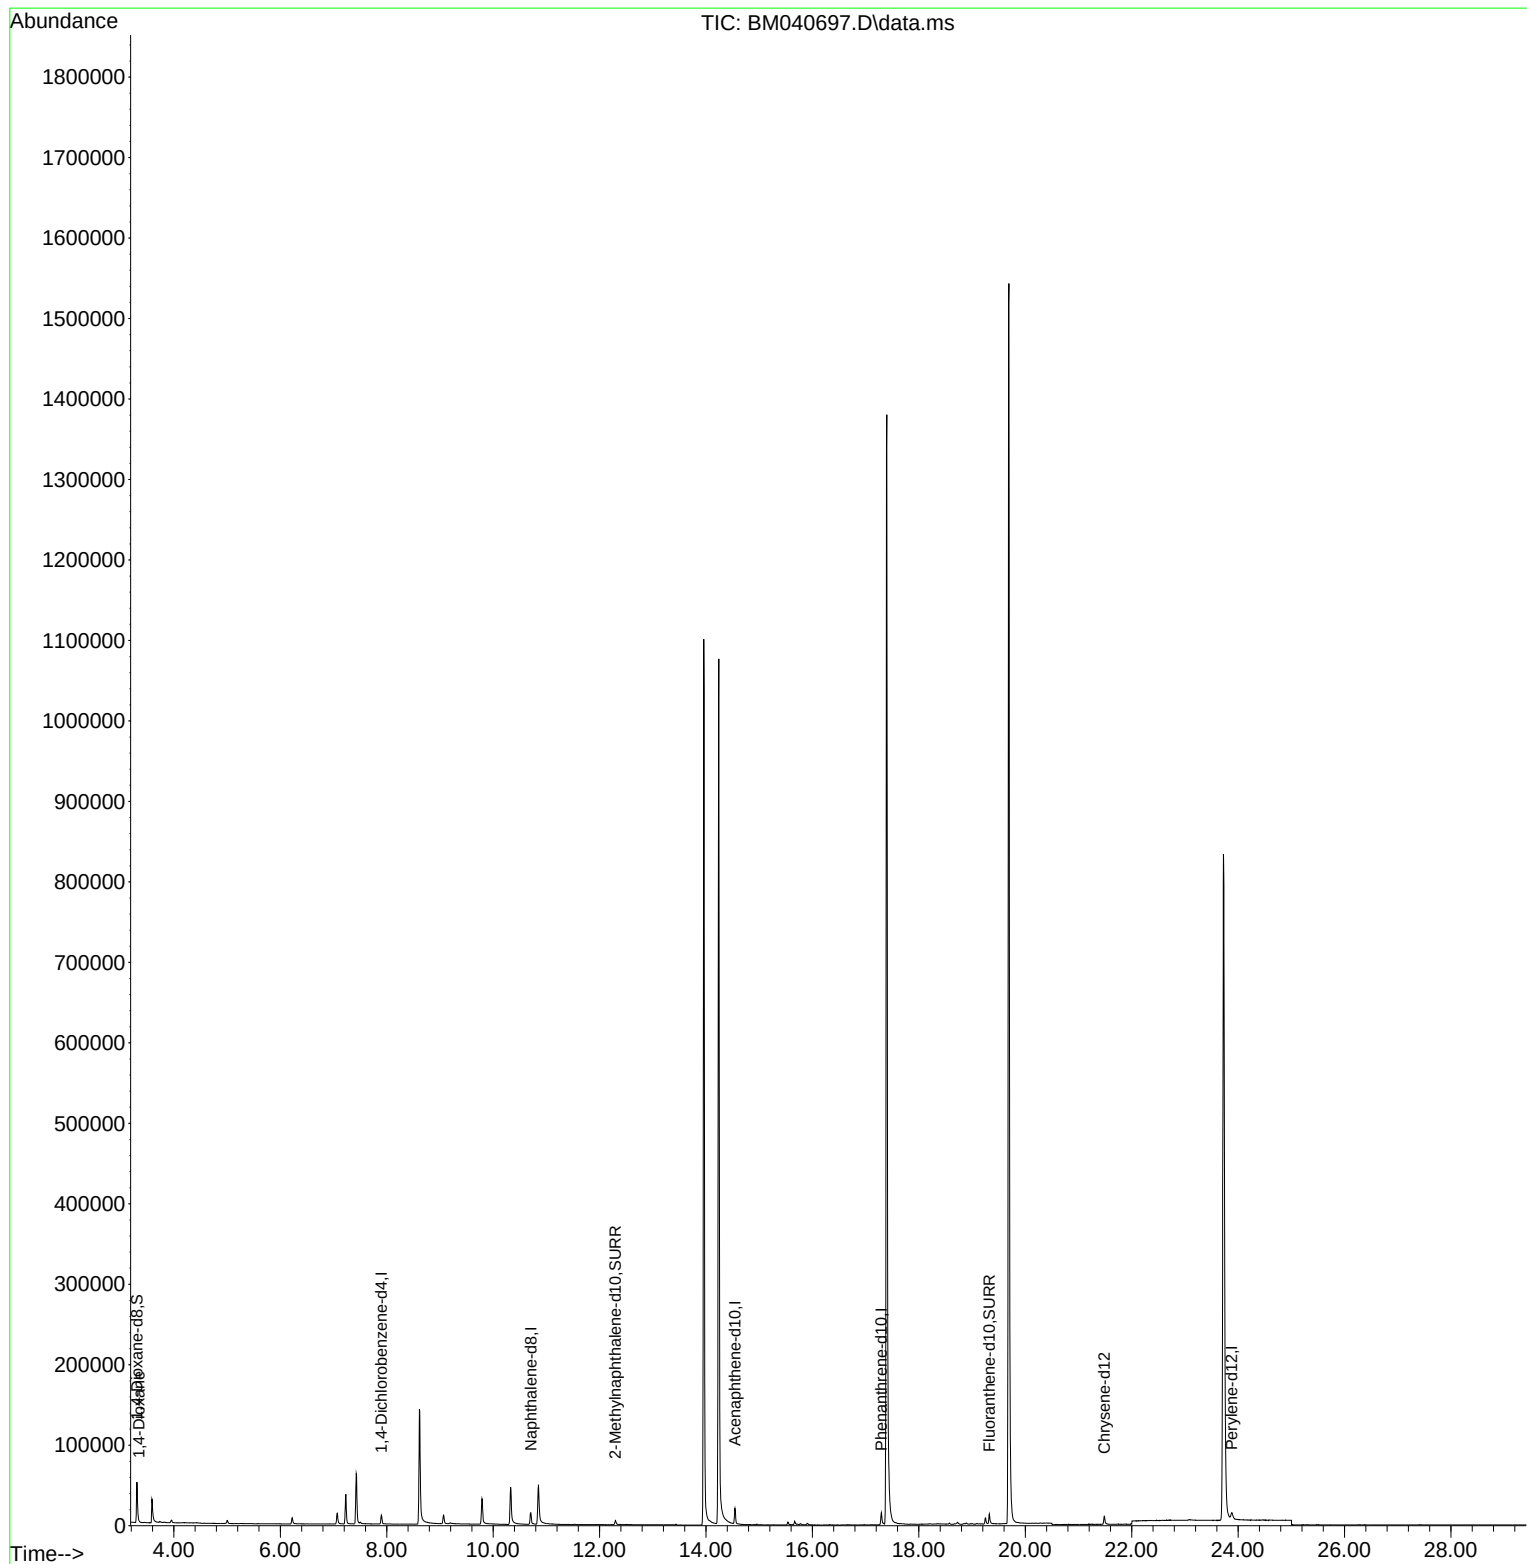

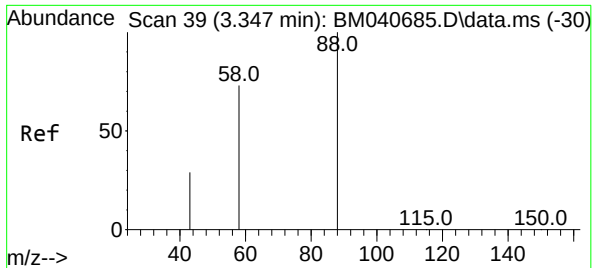

#2
 1,4-Dioxane
 Concen: 0.040 ng/ul
 RT: 3.343 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: BM040697.D
 Acq: 07 Jul 2023 03:51

Instrument :
 BNA_M
 ClientSampleId :
 DCGW2

Tgt Ion: 88 Resp: 379
 Ion Ratio Lower Upper
 88 100
 43 123.6 36.1 54.1#
 58 32.0 49.8 74.8#

