

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040703.D
 Acq On : 07 Jul 2023 08:12
 Operator : MA/JU
 Sample : 03283-04
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXYW8

Quant Time: Jul 07 08:52:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 09:30:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	6398	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.702	136	23185	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.541	164	12009	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.291	188	20173	0.400	ng/ul	-0.02
17) Chrysene-d12	21.486	240	11318	0.400	ng/ul	0.00
23) Perylene-d12	23.880	264	13596	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	36117	3.594	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.297	152	7404	0.228	ng/ul	-0.01
18) Fluoranthene-d10	19.325	212	10776	0.297	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.343	88	575	0.056	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040703.D
Acq On : 07 Jul 2023 08:12
Operator : MA/JU
Sample : 03283-04
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXYW8

Quant Time: Jul 07 08:52:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 09:30:35 2023
Response via : Initial Calibration

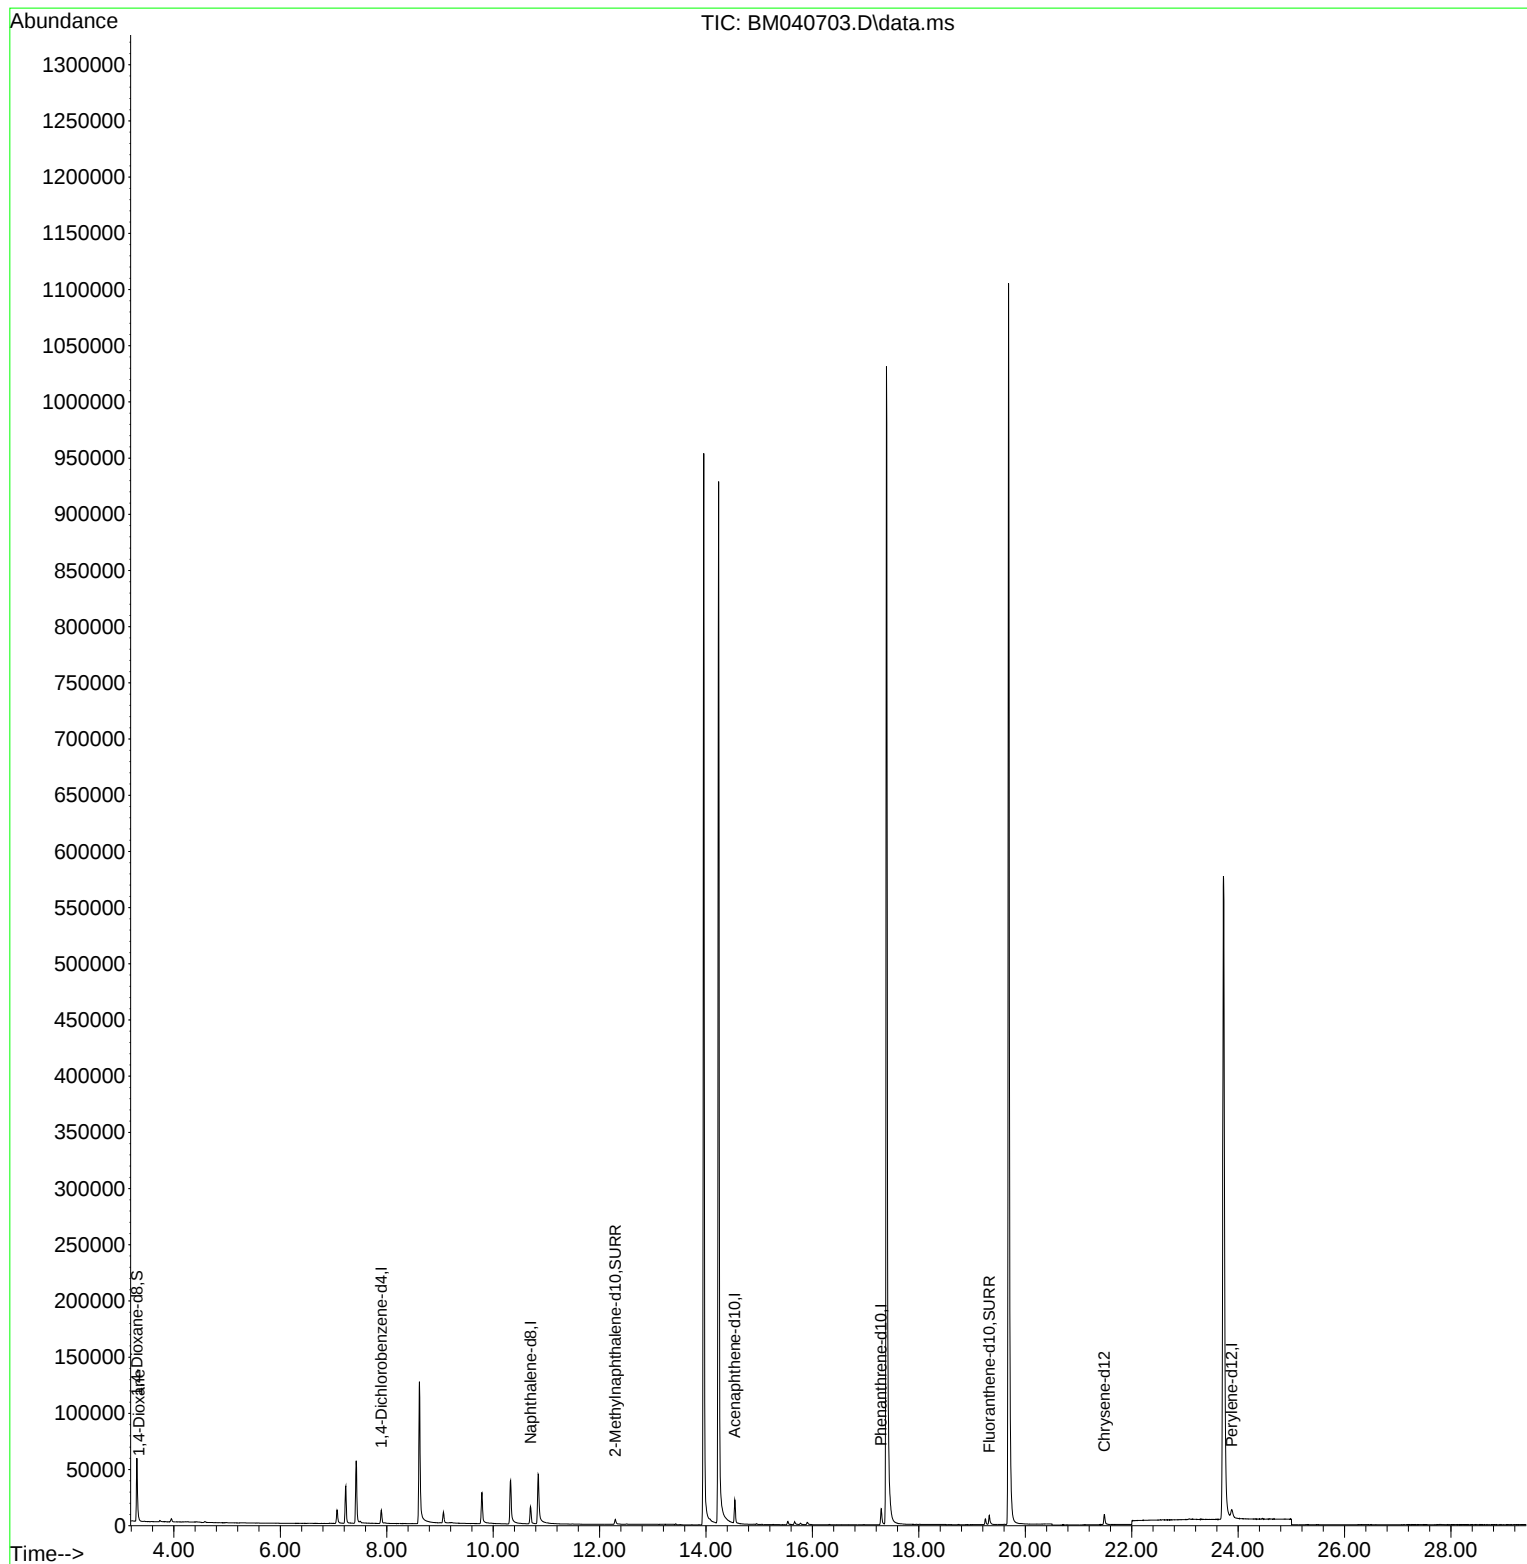

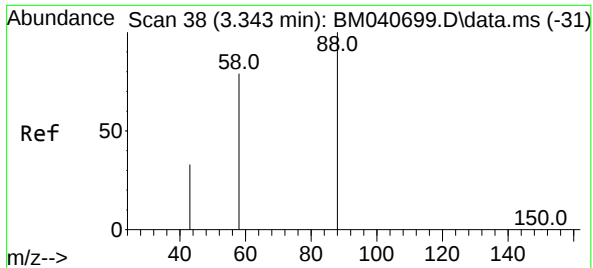

#2
 1,4-Dioxane
 Concen: 0.056 ng/ul
 RT: 3.343 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: BM040703.D
 Acq: 07 Jul 2023 08:12

Instrument :
 BNA_M
 ClientSampleId :
 EXYW8

Tgt Ion: 88 Resp: 575
 Ion Ratio Lower Upper
 88 100
 43 104.3 36.1 54.1#
 58 40.6 49.8 74.8#

