

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040704.D
 Acq On : 07 Jul 2023 08:49
 Operator : MA/JU
 Sample : 03283-05
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXYX1

Quant Time: Jul 07 09:23:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 09:30:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	6329	0.400	ng/u1	-0.01
4) Naphthalene-d8	10.702	136	22478	0.400	ng/u1	#-0.01
9) Acenaphthene-d10	14.541	164	11807	0.400	ng/u1	#-0.02
13) Phenanthrene-d10	17.291	188	19449	0.400	ng/u1	-0.02
17) Chrysene-d12	21.483	240	10723	0.400	ng/u1	-0.01
23) Perylene-d12	23.880	264	12887	0.400	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	37671	3.789	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.297	152	10247	0.325	ng/u1	-0.01
18) Fluoranthene-d10	19.324	212	14855	0.432	ng/u1	-0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.343	88	15441	1.526	ng/u1	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040704.D
Acq On : 07 Jul 2023 08:49
Operator : MA/JU
Sample : 03283-05
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXYX1


Quant Time: Jul 07 09:23:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 09:30:35 2023
Response via : Initial Calibration

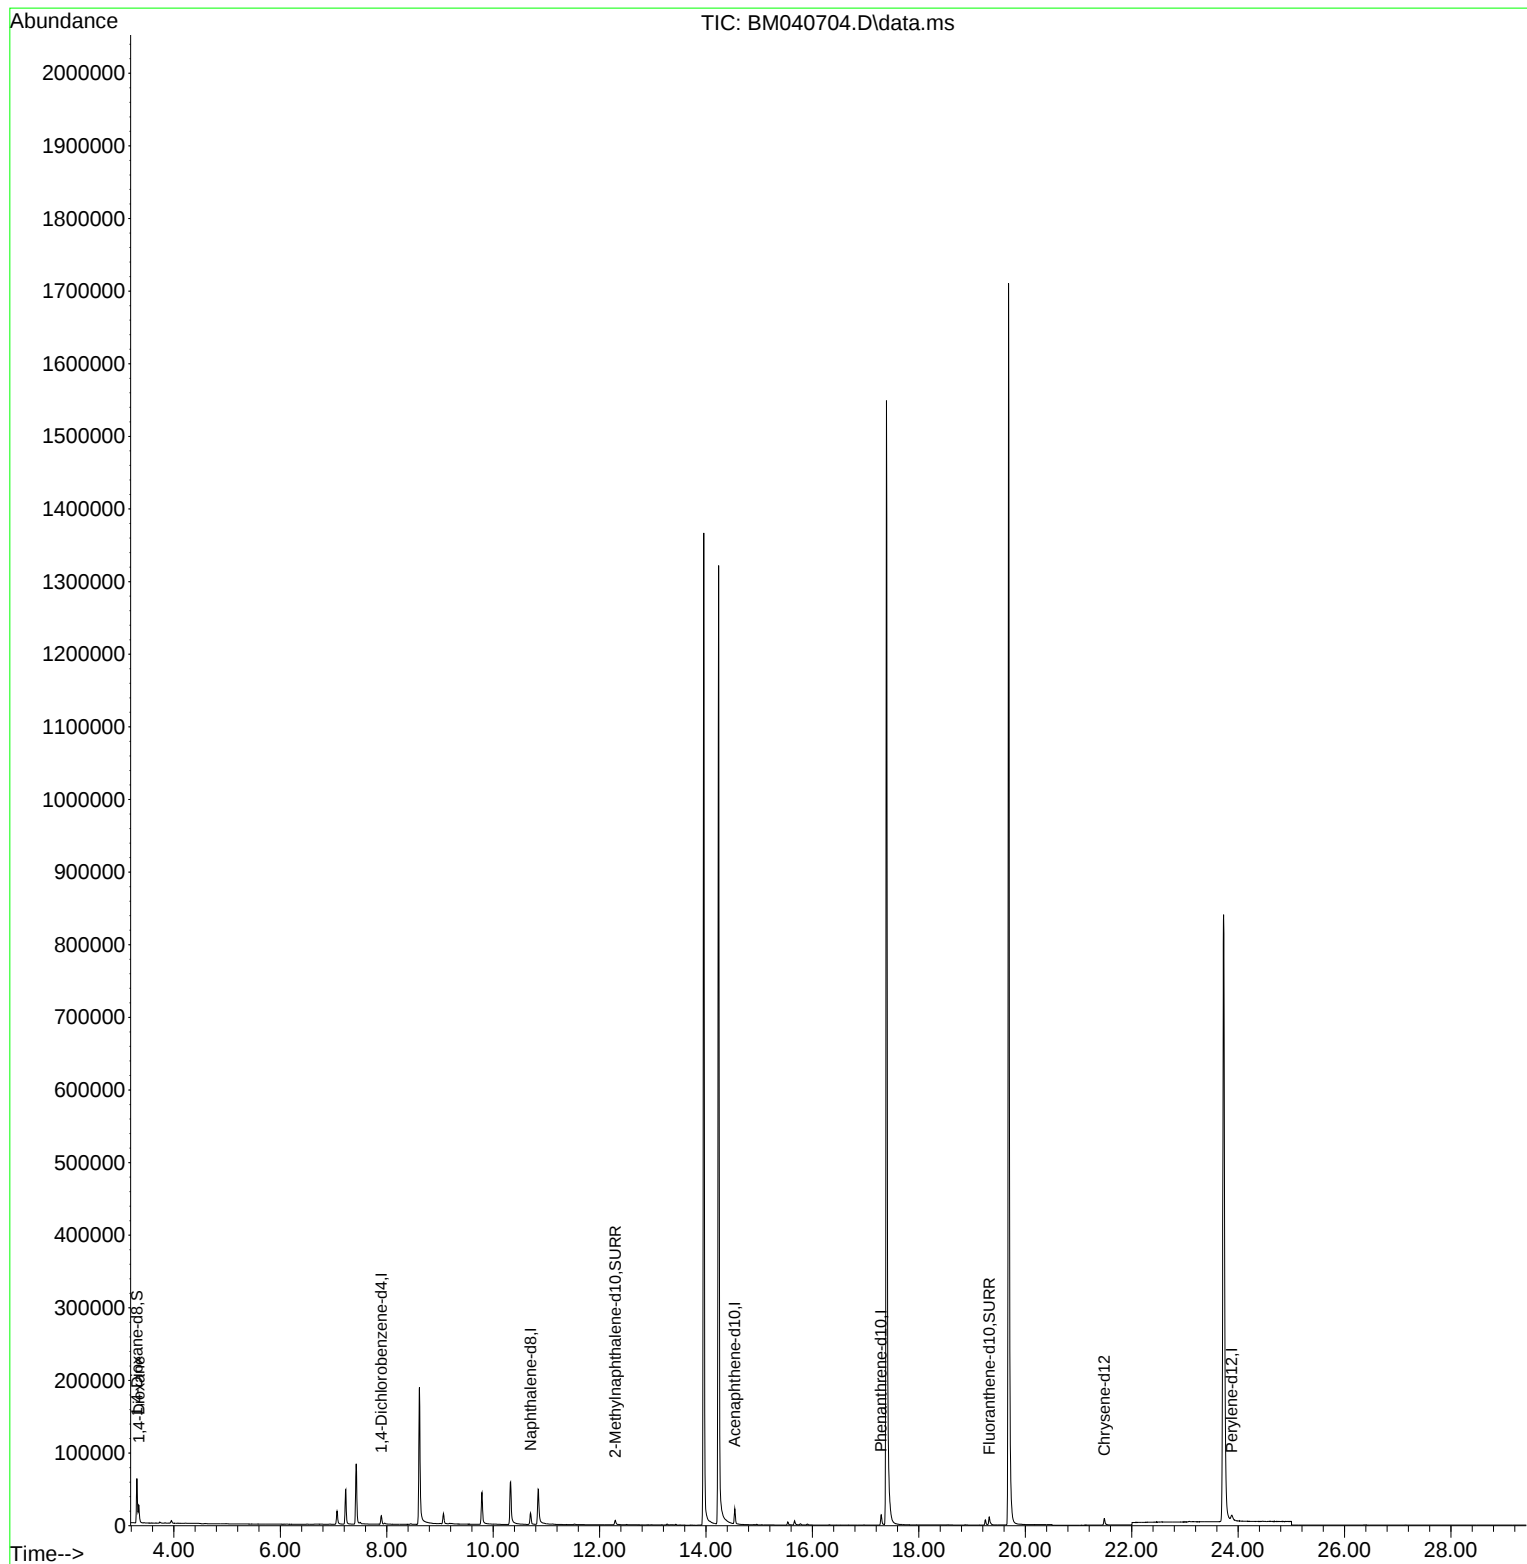

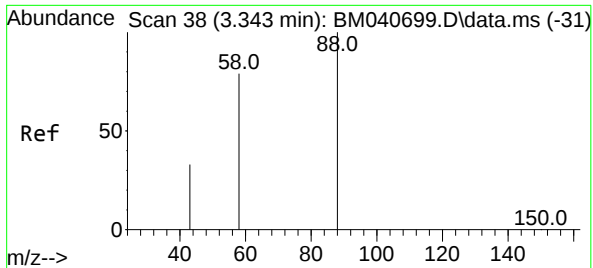

#2
 1,4-Dioxane
 Concen: 1.526 ng/ul
 RT: 3.343 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: BM040704.D
 Acq: 07 Jul 2023 08:49

Instrument :
 BNA_M
 ClientSampleId :
 EXYX1

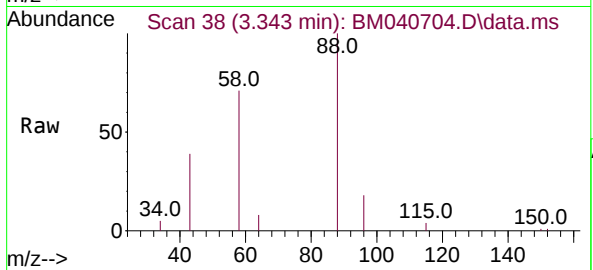

Tgt Ion: 88 Resp: 15441
 Ion Ratio Lower Upper
 88 100
 43 38.7 36.1 54.1
 58 70.8 49.8 74.8

