

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040717.D
 Acq On : 07 Jul 2023 17:01
 Operator : MA/JU
 Sample : 03283-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXYW9

Quant Time: Jul 07 20:04:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 10:22:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	4773	0.400	ng/ul	0.00
4) Naphthalene-d8	10.702	136	17503	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.541	164	9608	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.295	188	17220	0.400	ng/ul	0.00
17) Chrysene-d12	21.483	240	10008	0.400	ng/ul	0.00
23) Perylene-d12	23.877	264	10950	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	27973	3.731	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.297	152	7992	0.326	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	13831	0.431	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.338	88	35987	4.716	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040717.D
Acq On : 07 Jul 2023 17:01
Operator : MA/JU
Sample : 03283-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXYW9

Quant Time: Jul 07 20:04:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 10:22:24 2023
Response via : Initial Calibration

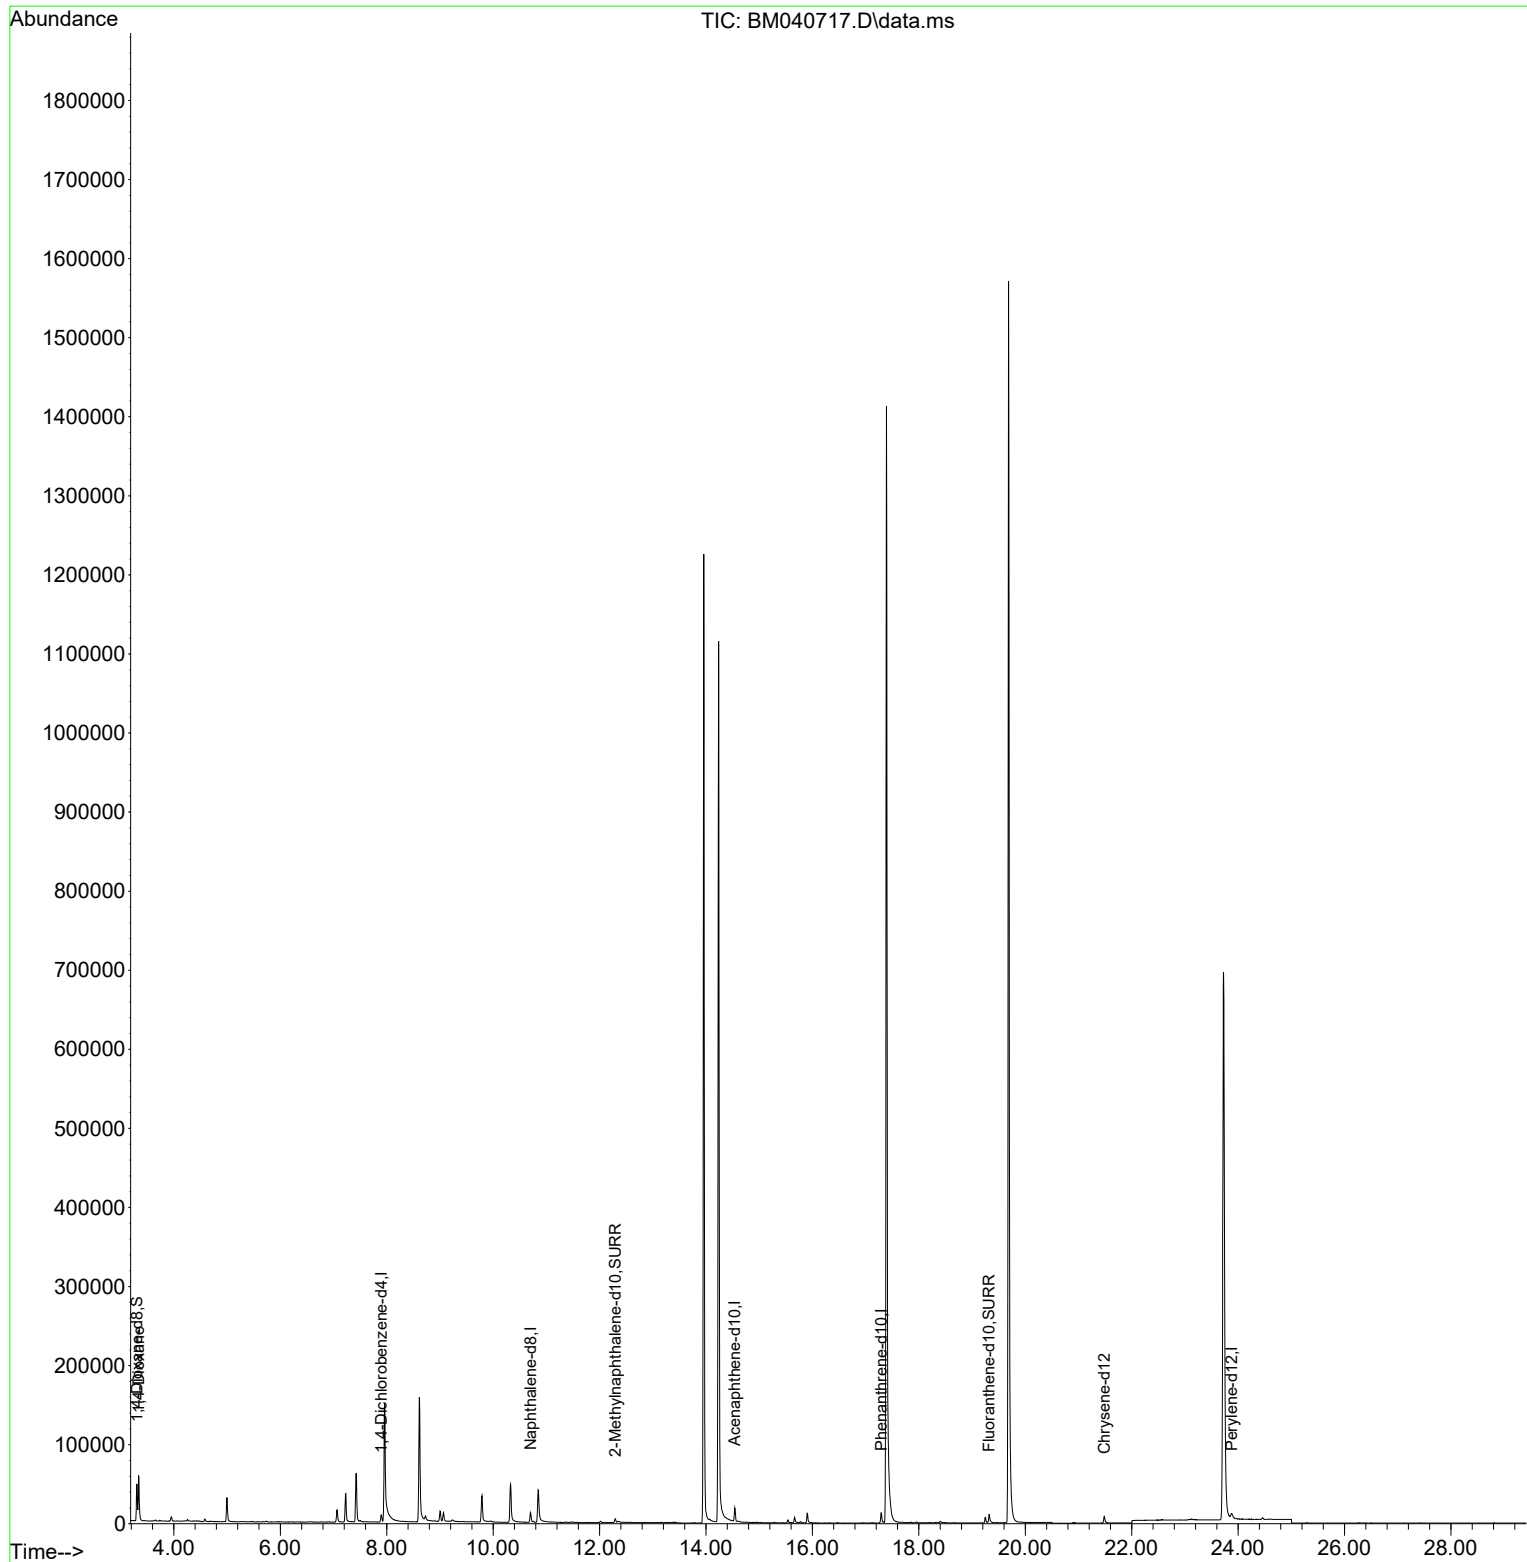

Abundance Scan 38 (3.343 min): BM040711.D\data.ms (-31)

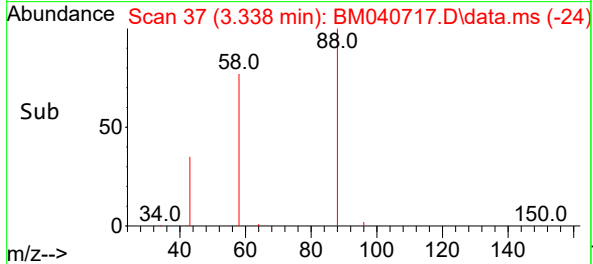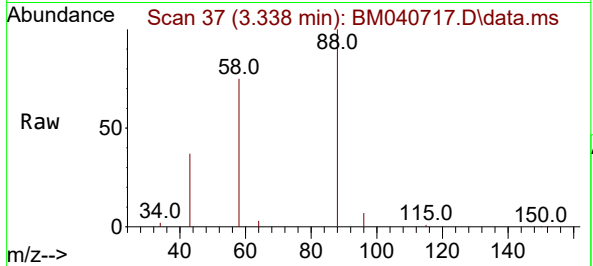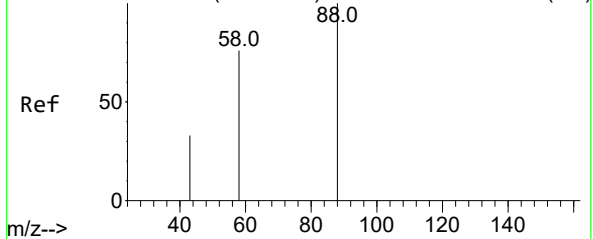

#2
1,4-Dioxane
Concen: 4.716 ng/ul
RT: 3.338 min Scan# 31
Delta R.T. -0.004 min
Lab File: BM040717.D
Acq: 07 Jul 2023 17:01

Instrument :
BNA_M
ClientSampleId :
EXYW9

Tgt Ion: 88 Resp: 35987
Ion Ratio Lower Upper
88 100
43 37.3 36.1 54.1
58 74.9 49.8 74.8#

