

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040719.D
 Acq On : 07 Jul 2023 18:16
 Operator : MA/JU
 Sample : 03283-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXYZ0

Quant Time: Jul 07 20:06:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 10:22:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.895	152	4311	0.400	ng/ul	0.00
4) Naphthalene-d8	10.702	136	16139	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.541	164	8904	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.291	188	17009	0.400	ng/ul	0.00
17) Chrysene-d12	21.483	240	10387	0.400	ng/ul	0.00
23) Perylene-d12	23.877	264	11392	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	23920	3.532	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	6396	0.283	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	13211	0.397	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.339	88	1005	0.146	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040719.D
Acq On : 07 Jul 2023 18:16
Operator : MA/JU
Sample : 03283-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXYZ0


Quant Time: Jul 07 20:06:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 10:22:24 2023
Response via : Initial Calibration

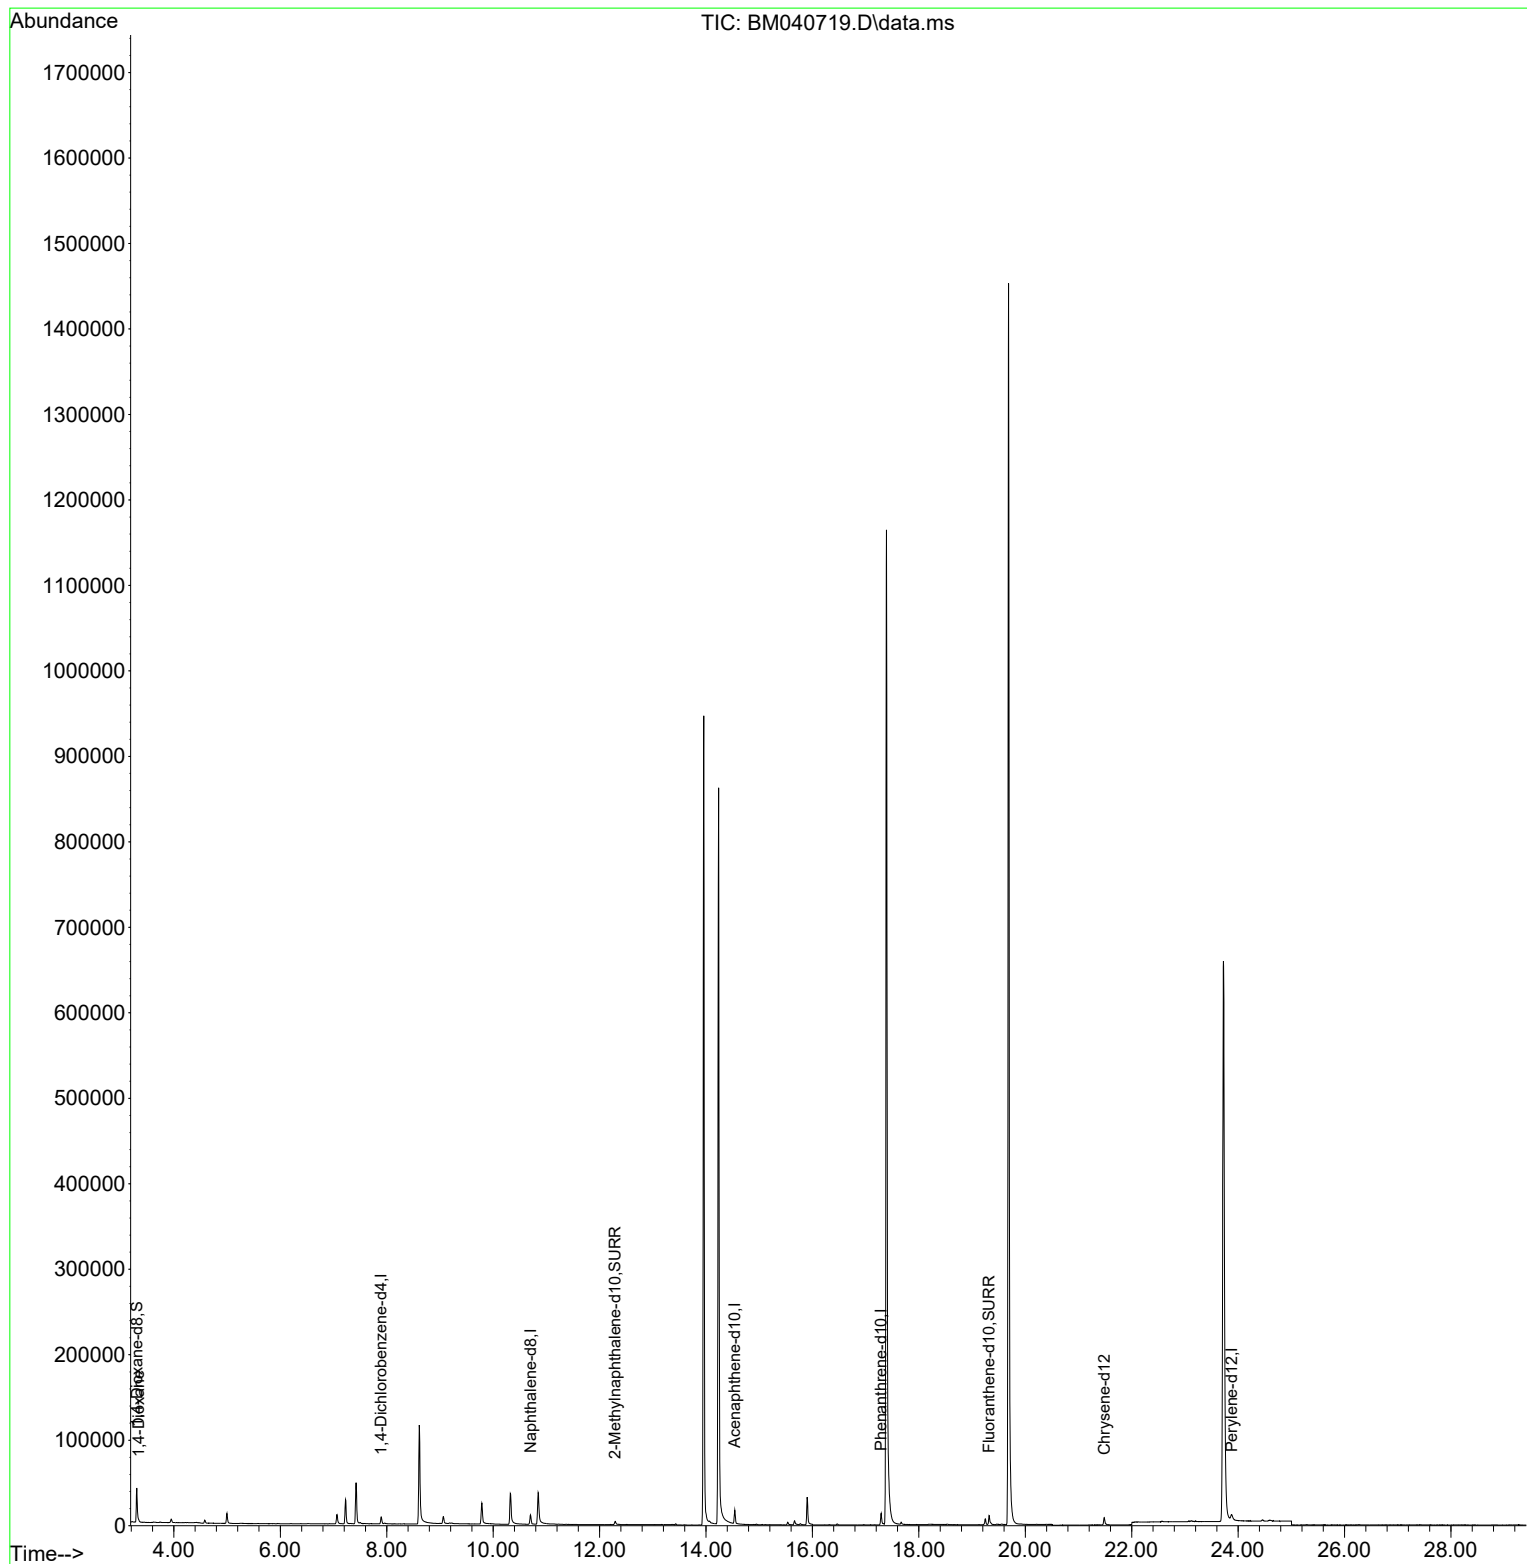

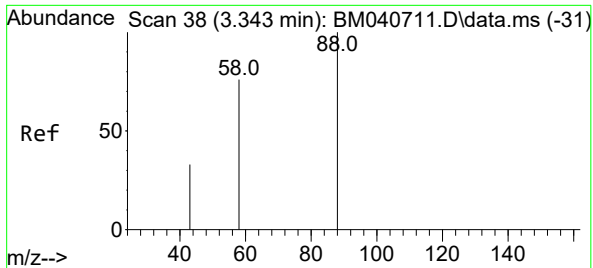

#2
 1,4-Dioxane
 Concen: 0.146 ng/ul
 RT: 3.339 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BM040719.D
 Acq: 07 Jul 2023 18:16

Instrument :
 BNA_M
 ClientSampleId :
 EXYZ0

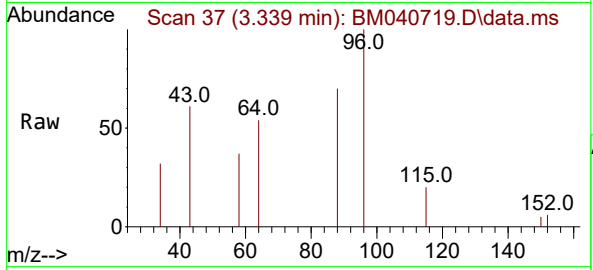

Tgt Ion: 88 Resp: 1005

Ion	Ratio	Lower	Upper
88	100		
43	87.3	36.1	54.1#
58	52.8	49.8	74.8

