

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040721.D
 Acq On : 07 Jul 2023 19:32
 Operator : MA/JU
 Sample : 03284-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCGZ5

Quant Time: Jul 07 20:08:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 10:22:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	5490	0.400	ng/ul	0.00
4) Naphthalene-d8	10.702	136	20422	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.541	164	11041	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.295	188	21853	0.400	ng/ul	0.00
17) Chrysene-d12	21.480	240	12776	0.400	ng/ul	0.00
23) Perylene-d12	23.877	264	13209	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	34032	3.946	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.291	152	8183	0.286	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	16059	0.392	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.339	88	6278	0.715	ng/ul	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040721.D
Acq On : 07 Jul 2023 19:32
Operator : MA/JU
Sample : 03284-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCGZ5


Quant Time: Jul 07 20:08:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 10:22:24 2023
Response via : Initial Calibration

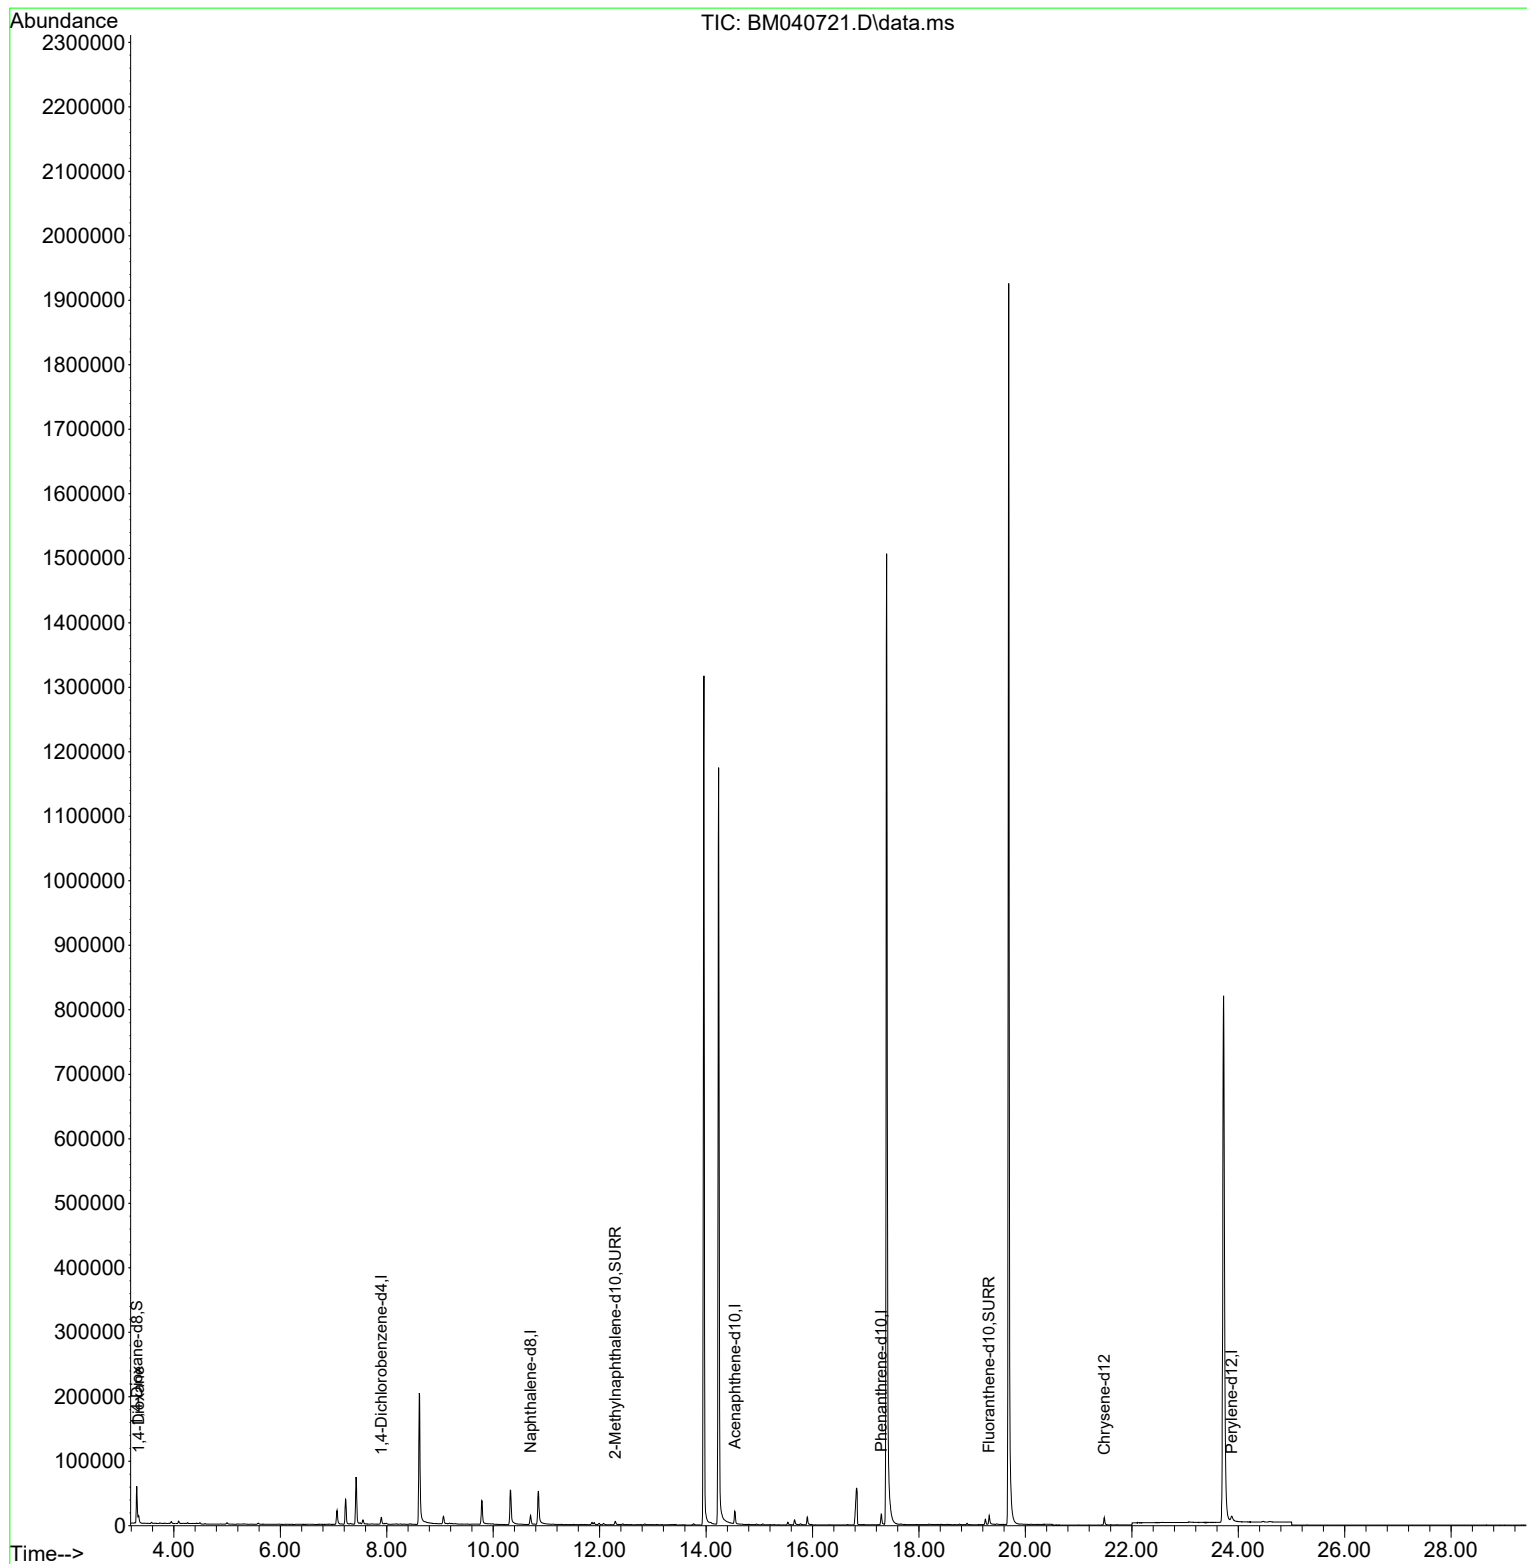


Abundance Scan 38 (3.343 min): BM040711.D\data.ms (-31)

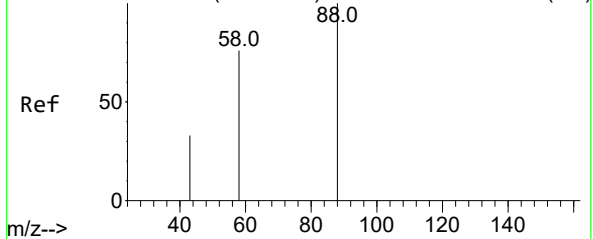

Abundance Scan 37 (3.339 min): BM040721.D\data.ms

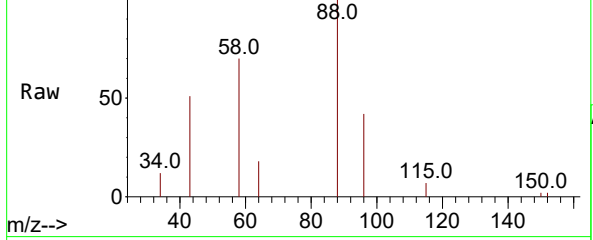

Abundance Scan 37 (3.339 min): BM040721.D\data.ms (-24)

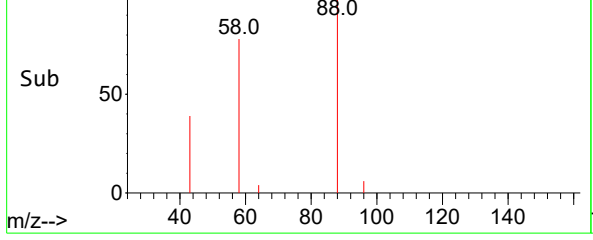

#2
1,4-Dioxane
Concen: 0.715 ng/ul
RT: 3.339 min Scan# 31
Delta R.T. -0.004 min
Lab File: BM040721.D
Acq: 07 Jul 2023 19:32

Instrument :
BNA_M
ClientSampleId :
DCGZ5

Tgt Ion:	88	Resp:	6278
Ion	Ratio	Lower	Upper
88	100		
43	51.3	36.1	54.1
58	69.6	49.8	74.8

