

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
 Data File : BM040722.D
 Acq On : 07 Jul 2023 20:10
 Operator : MA/JU
 Sample : 03284-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCGZ7

Quant Time: Jul 07 20:49:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 10:22:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.895	152	5199	0.400	ng/ul	0.00
4) Naphthalene-d8	10.702	136	19666	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.541	164	11013	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.291	188	20384	0.400	ng/ul	0.00
17) Chrysene-d12	21.483	240	12014	0.400	ng/ul	0.00
23) Perylene-d12	23.880	264	12812	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	34615	4.239	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.297	152	10338	0.375	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	17888	0.464	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.339	88	662	0.080	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070523\
Data File : BM040722.D
Acq On : 07 Jul 2023 20:10
Operator : MA/JU
Sample : 03284-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCGZ7

Quant Time: Jul 07 20:49:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 10:22:24 2023
Response via : Initial Calibration

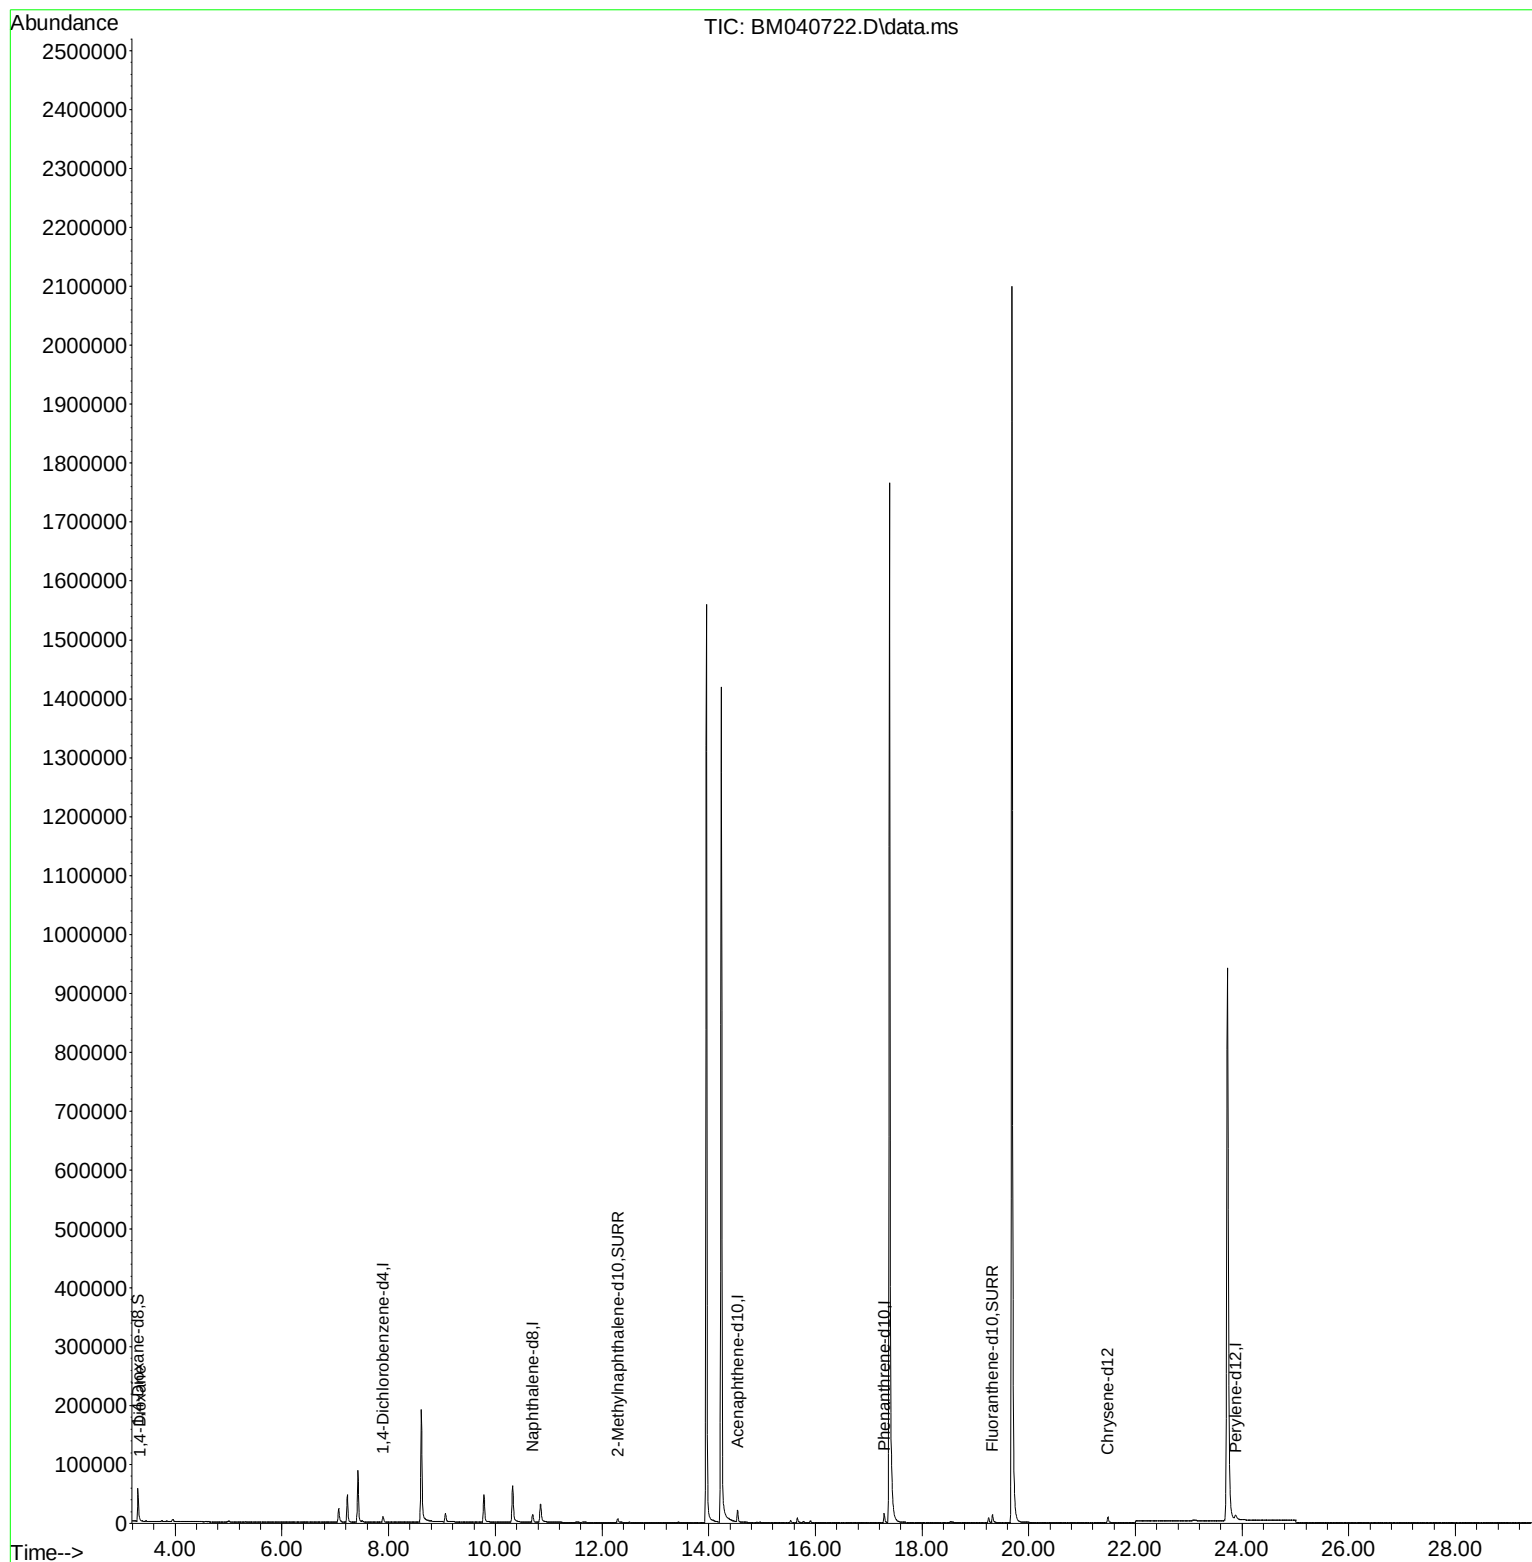

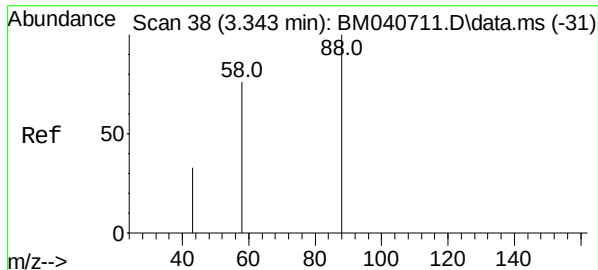

1,4-Dioxane
 Concen: 0.080 ng/ul
 RT: 3.339 min Scan# 1
 Delta R.T. -0.004 min
 Lab File: BM040722.D
 Acq: 07 Jul 2023 20:10

Instrument :
 BNA_M
 ClientSampleId :
 DCGZ7

Tgt Ion: 88 Resp: 662
 Ion Ratio Lower Upper
 88 100
 43 93.8 36.1 54.1#
 58 42.9 49.8 74.8#

