

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070618\
 Data File : BM015812.D
 Acq On : 06 Jul 2018 21:21
 Operator : SJ/JU
 Sample : J3845-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GF-02

Quant Time: Jul 07 01:31:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 05 17:39:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.30	152	116086	20.00	ng	-0.01
21) Naphthalene-d8	11.13	136	464506	20.00	ng	-0.01
38) Acenaphthene-d10	14.93	164	257414	20.00	ng	0.00
63) Phenanthrene-d10	17.65	188	523633	20.00	ng	0.00
75) Chrysene-d12	21.76	240	383563	20.00	ng	-0.01
86) Perylene-d12	24.16	264	343084	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.81	112	1097781	162.18	ng	0.00
7) Phenol-d6	7.46	99	1453808	156.88	ng	0.00
23) Nitrobenzene-d5	9.50	82	974087	102.32	ng	0.00
41) 2,4,6-Tribromophenol	16.40	330	539843	160.50	ng	-0.01
44) 2-Fluorobiphenyl	13.55	172	2107722	101.65	ng	-0.01
78) Terphenyl-d14	20.22	244	2718678	131.47	ng	0.00
Target Compounds						
10) Phenol	7.49	94	32575	3.498	ng	87
49) Dimethylphthalate	14.37	163	339181	14.940	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070618\
Data File : BM015812.D
Acq On : 06 Jul 2018 21:21
Operator : SJ/JU
Sample : J3845-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GF-02

Quant Time: Jul 07 01:31:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 05 17:39:50 2018
Response via : Initial Calibration

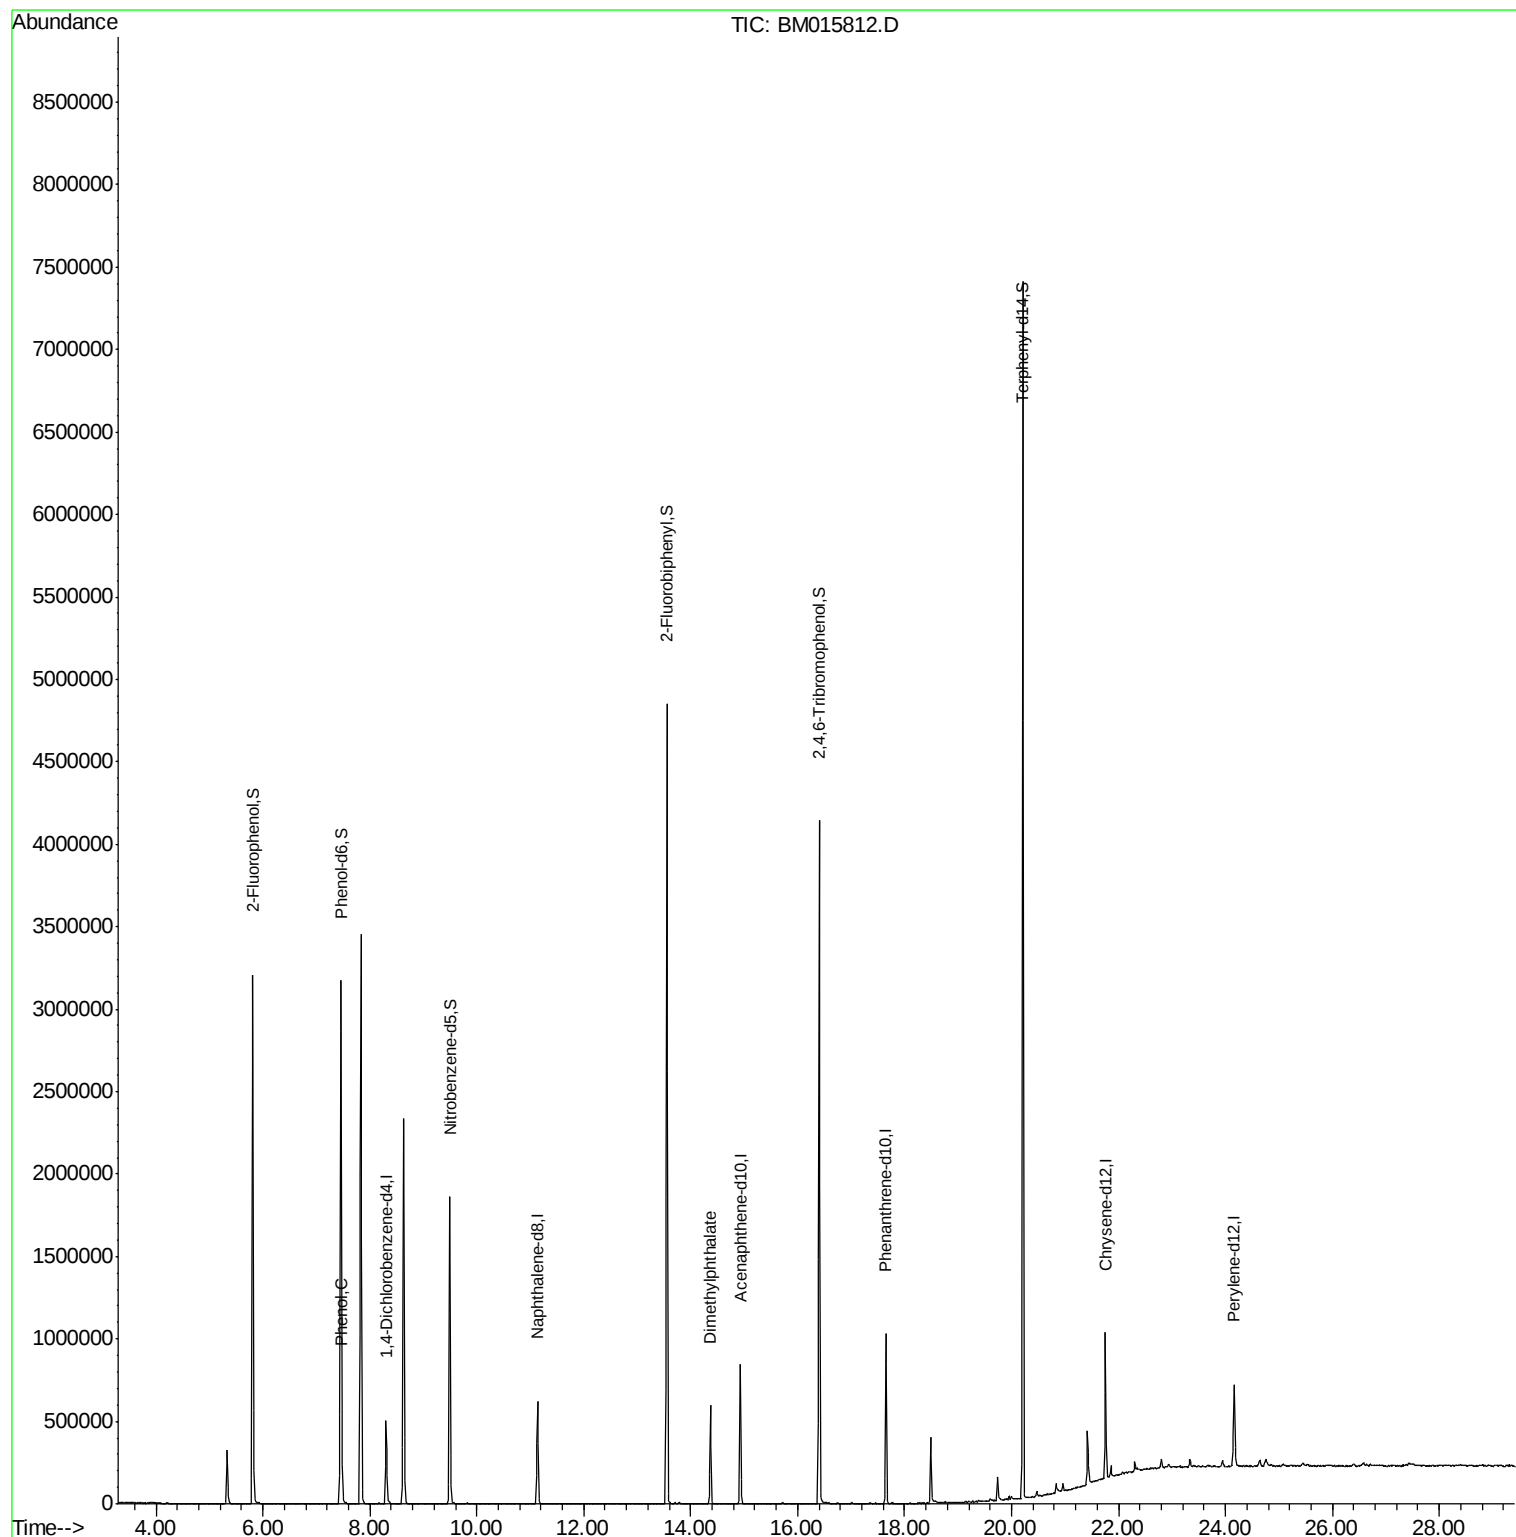


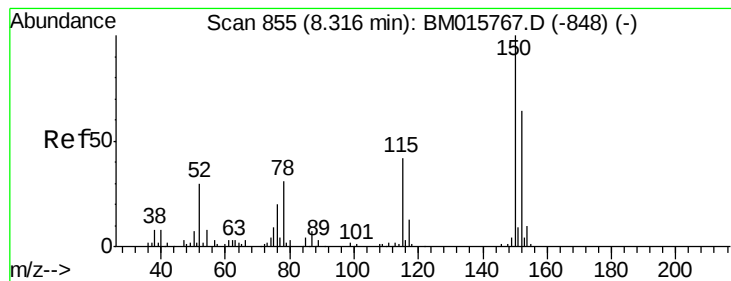




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.30 min Scan# 853
 Delta R.T. -0.01 min
 Lab File: BM015812.D
 Acq: 06 Jul 2018 21:21

Instrument :
 BNA_M
 ClientSampleId :
 GF-02

Tgt Ion:152 Resp: 116086
 Ion Ratio Lower Upper
 152 100
 150 164.2 119.5 179.3
 115 65.9 43.0 64.4#

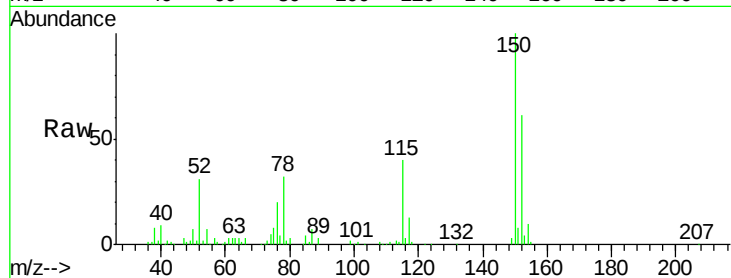


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

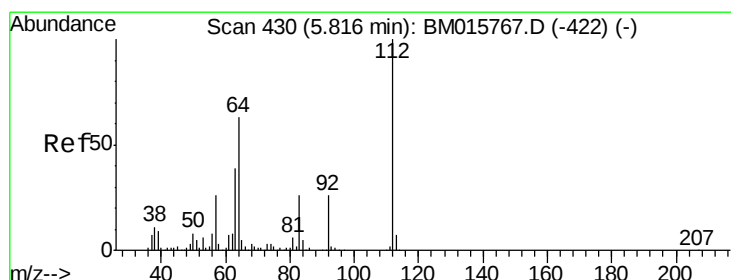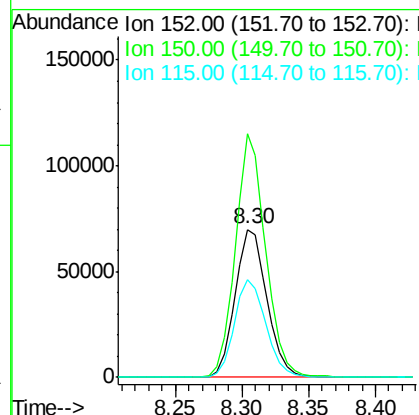
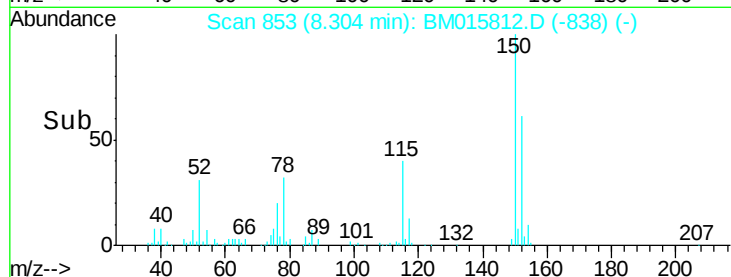





#5
 2-Fluorophenol
 Concen: Below ng
 RT: 5.81 min Scan# 429
 Delta R.T. -0.01 min
 Lab File: BM015812.D
 Acq: 06 Jul 2018 21:21

Tgt Ion:112 Resp: 1097781
 Ion Ratio Lower Upper
 112 100
 64 63.0 38.6 57.8#
 63 40.2 19.3 28.9#

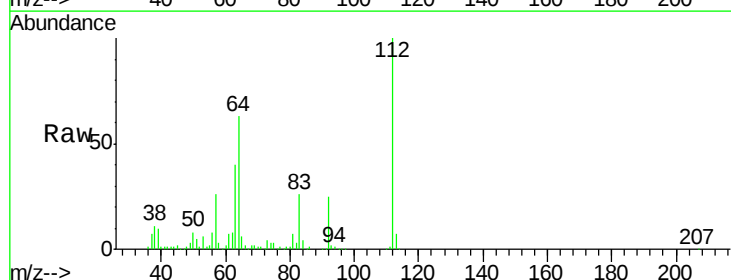

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BM0
 Ion 63.00 (62.70 to 63.70): BM0

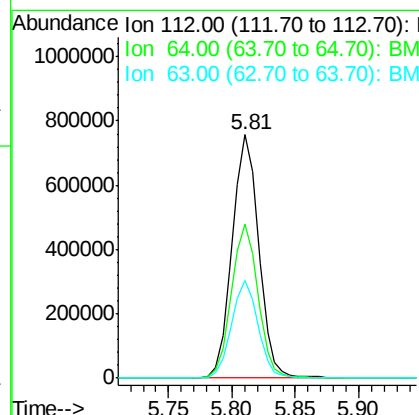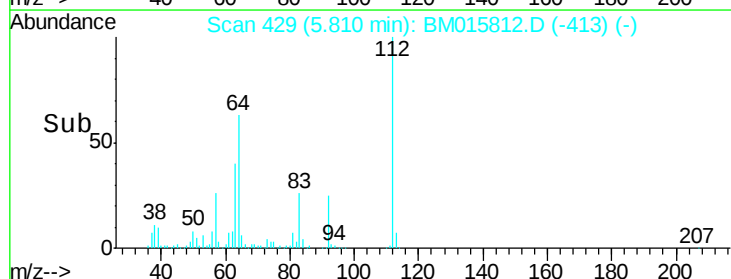

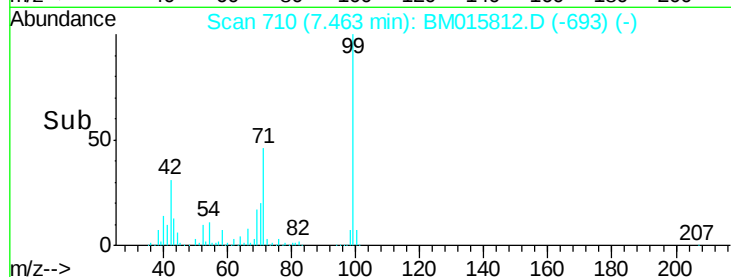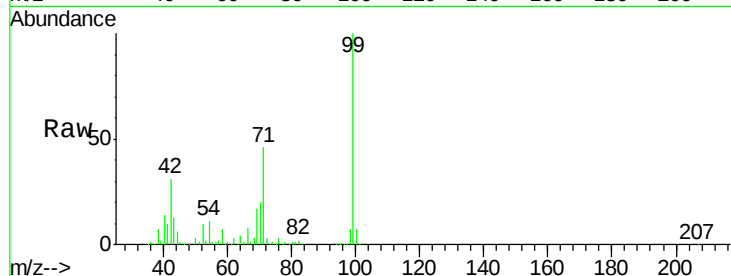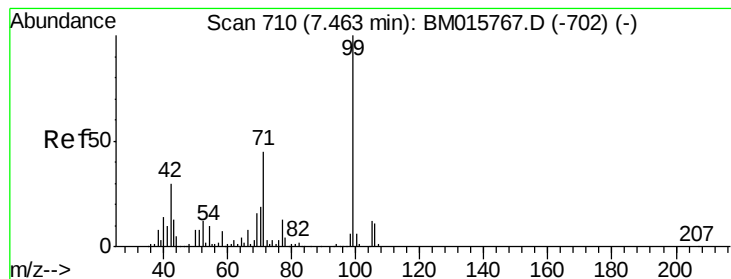

#7

Phenol-d6

Concen: N.D. ng

RT: 7.46 min Scan# 710

Delta R.T. -0.00 min

Lab File: BM015812.D

Acq: 06 Jul 2018 21:21

Instrument :

BNA_M

ClientSampled :

GF-02





Tgt Ion: 99 Resp: 1453808

Ion Ratio Lower Upper

99 100

42 30.7 11.0 16.4#

71 46.1 23.4 35.2#

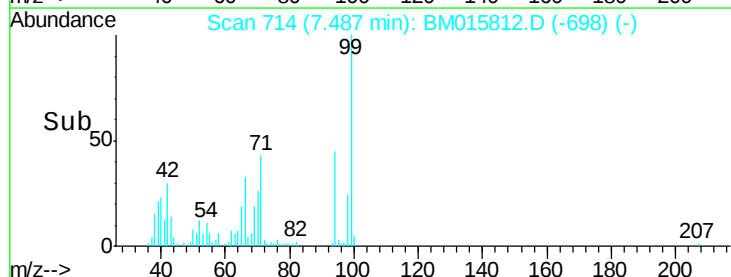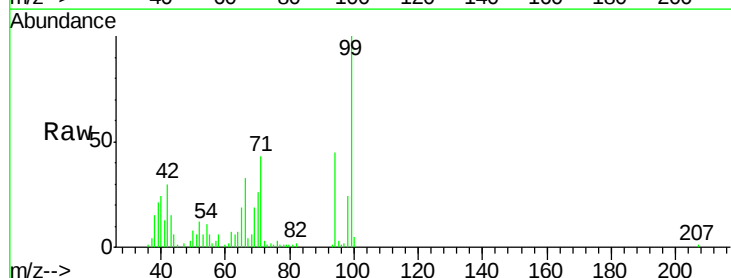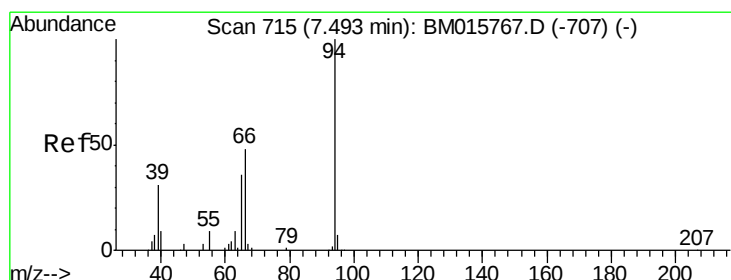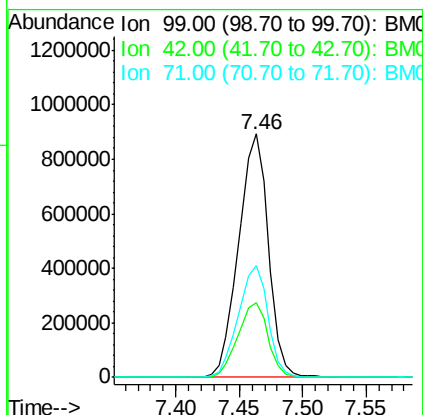

#10

Phenol

Concen: 3.498 ng

RT: 7.49 min Scan# 714

Delta R.T. -0.01 min

Lab File: BM015812.D

Acq: 06 Jul 2018 21:21


Tgt Ion: 94 Resp: 32575


Ion Ratio Lower Upper

94 100

65 42.9 18.8 58.8

66 72.5 39.9 79.9

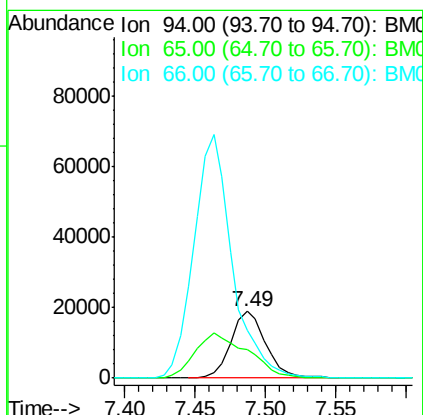


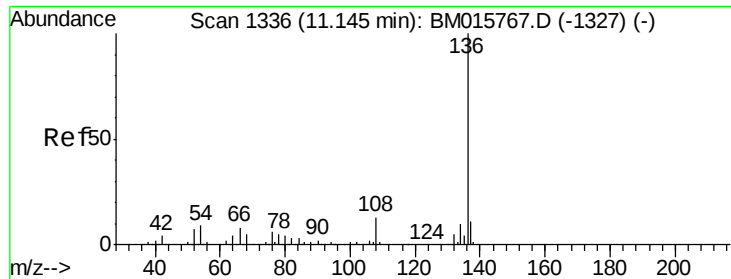




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.13 min Scan# 1334
Delta R.T. -0.01 min
Lab File: BM015812.D
Acq: 06 Jul 2018 21:21

Instrument :
BNA_M
ClientSampleId :
GF-02

Tgt Ion:	136	Resp:	464506
Ion	Ratio	Lower	Upper
136	100		
137	11.4	8.7	13.1
54	9.0	4.6	6.8#
68	4.8	3.7	5.5

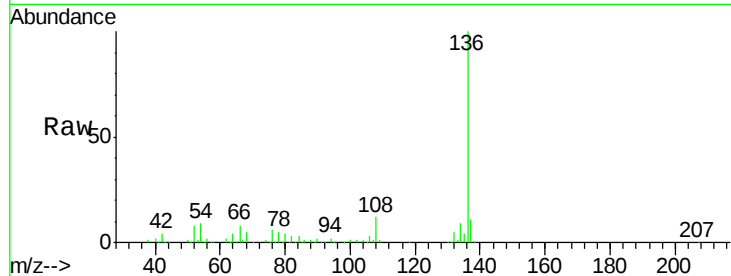


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

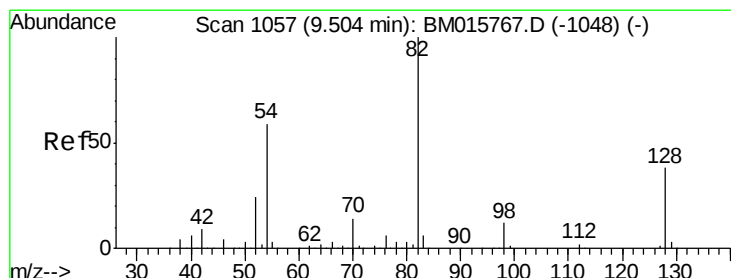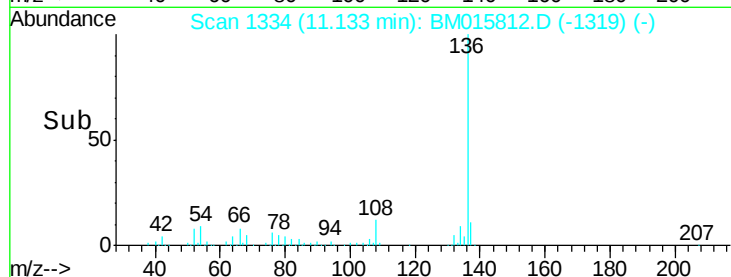
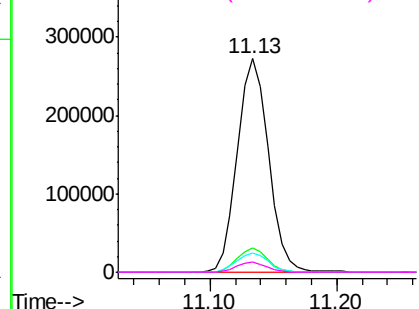



#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.50 min Scan# 1056
Delta R.T. -0.01 min
Lab File: BM015812.D
Acq: 06 Jul 2018 21:21

Tgt Ion:	82	Resp:	974087
Ion	Ratio	Lower	Upper
82	100		
128	38.8	32.8	49.2
54	60.8	40.6	60.8

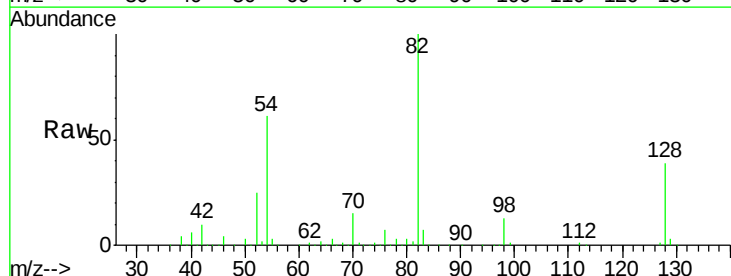

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

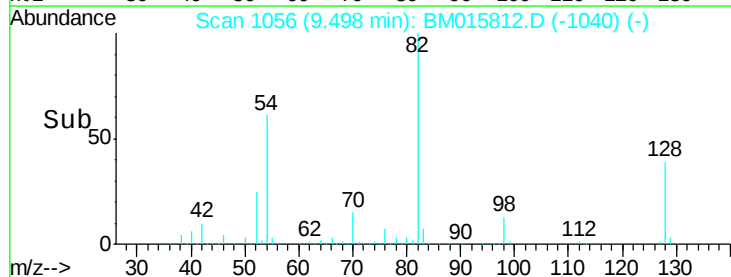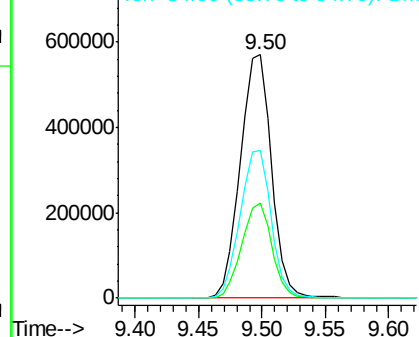


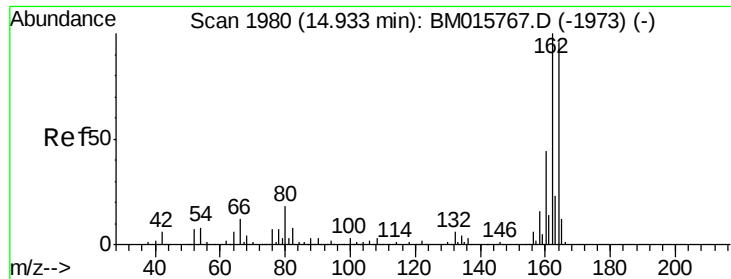




#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.93 min Scan# 1979
Delta R.T. -0.01 min
Lab File: BM015812.D
Acq: 06 Jul 2018 21:21

Instrument :
BNA_M
ClientSampleId :
GF-02

Tgt Ion:164 Resp: 257414
Ion Ratio Lower Upper
164 100
162 103.1 82.4 123.6
160 48.7 35.8 53.6

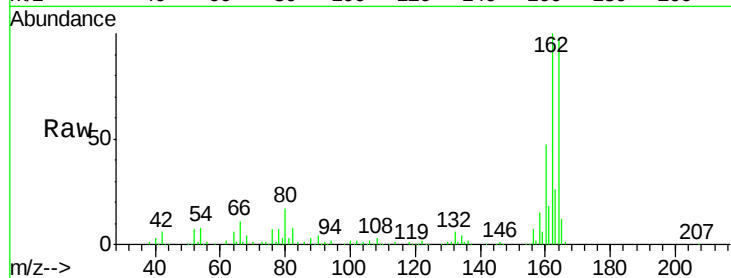


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

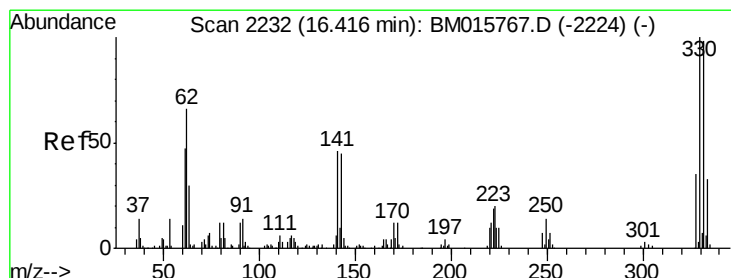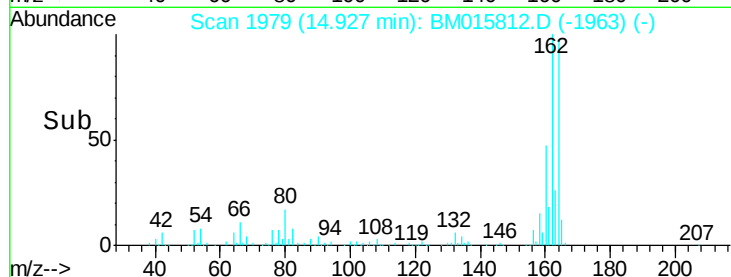
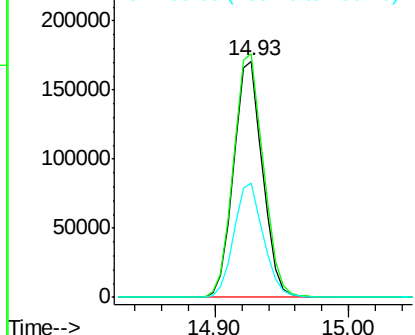



#41
2,4,6-Tribromophenol
Concen: N.D. ng
RT: 16.40 min Scan# 2230
Delta R.T. -0.01 min
Lab File: BM015812.D
Acq: 06 Jul 2018 21:21

Tgt Ion:330 Resp: 539843
Ion Ratio Lower Upper
330 100
332 95.9 0.0 0.0#
141 51.4 0.0 0.0#

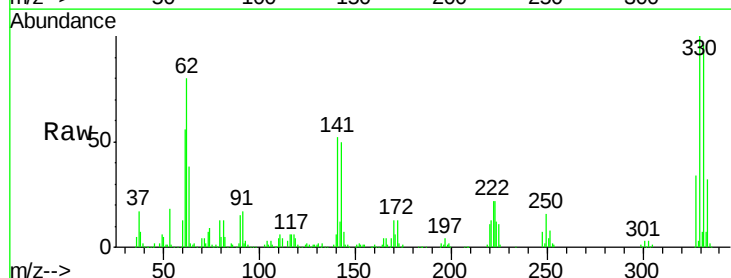

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



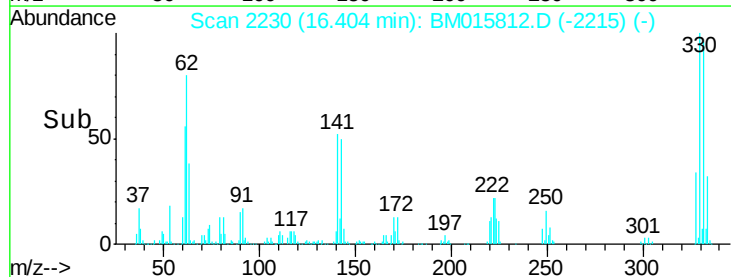
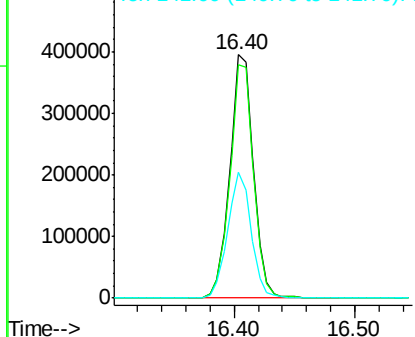


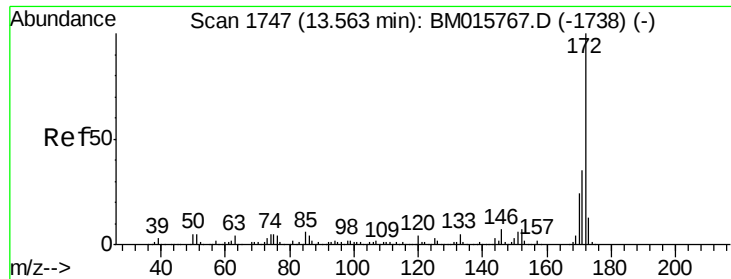

#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.55 min Scan# 1745
 Delta R.T. -0.01 min
 Lab File: BM015812.D
 Acq: 06 Jul 2018 21:21




Instrument :
 BNA_M
 ClientSampleId :
 GF-02


Tgt Ion:172 Resp: 2107722
 Ion Ratio Lower Upper
 172 100
 171 36.1 28.5 42.7
 170 23.8 18.8 28.2

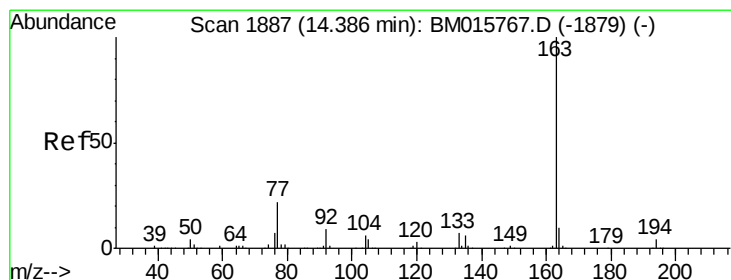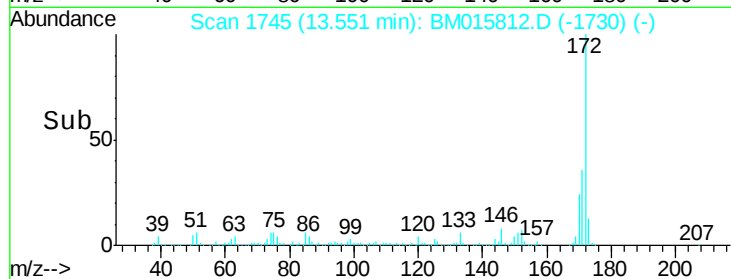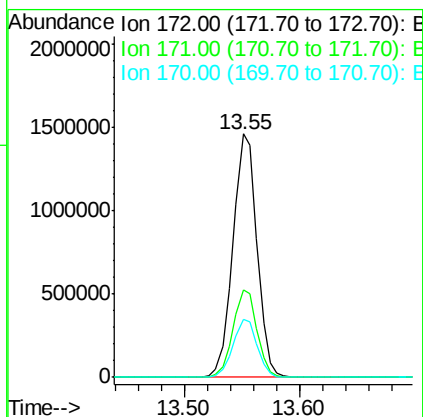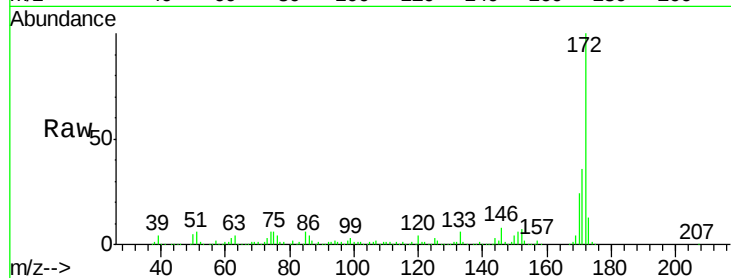

#49
 Dimethylphthalate
 Concen: 14.940 ng
 RT: 14.37 min Scan# 1884
 Delta R.T. -0.02 min
 Lab File: BM015812.D
 Acq: 06 Jul 2018 21:21

Tgt Ion:163 Resp: 339181
 Ion Ratio Lower Upper
 163 100
 194 3.3 2.7 4.1
 164 10.1 8.2 12.2


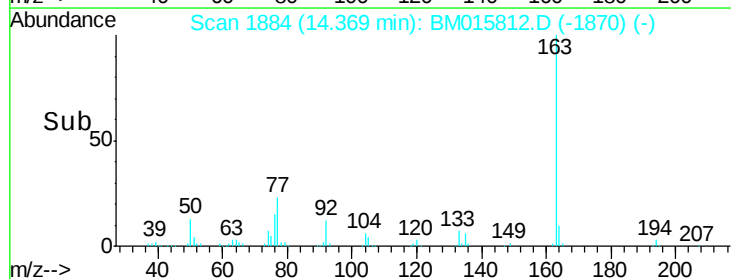
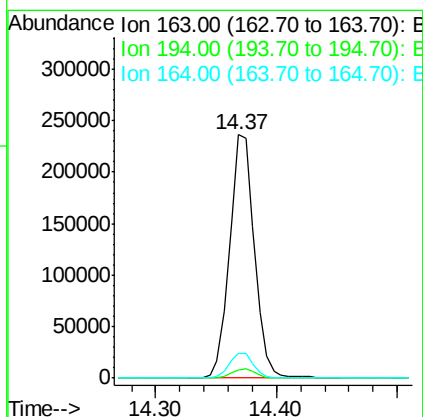
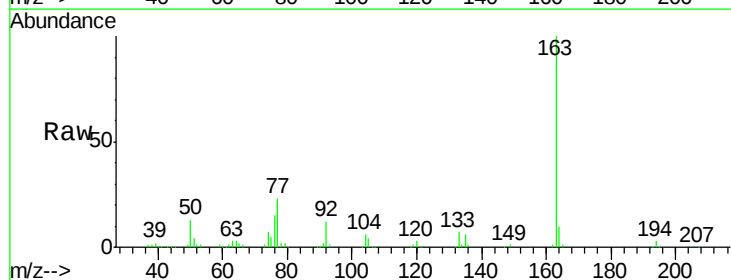


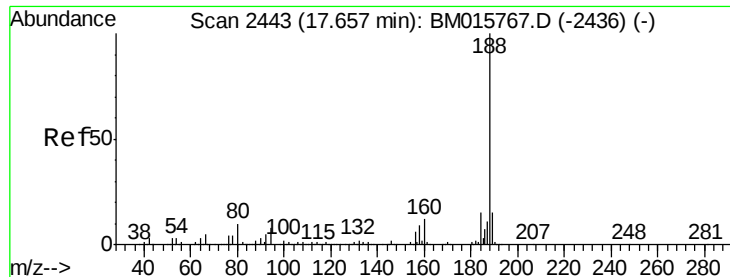

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.65 min Scan# 2442
Delta R.T. -0.01 min
Lab File: BM015812.D
Acq: 06 Jul 2018 21:21




Instrument :
BNA_M
ClientSampled :
GF-02


Tgt Ion:188 Resp: 523633
Ion Ratio Lower Upper
188 100
94 7.4 8.7 13.1#
80 8.6 9.3 13.9#

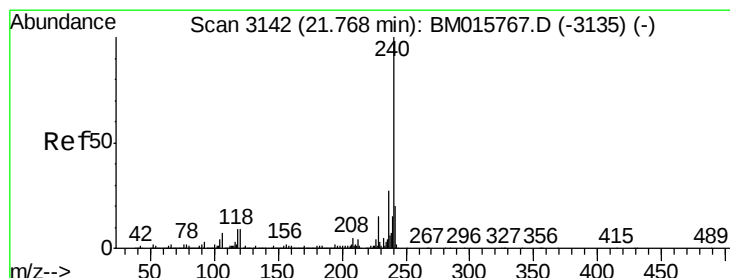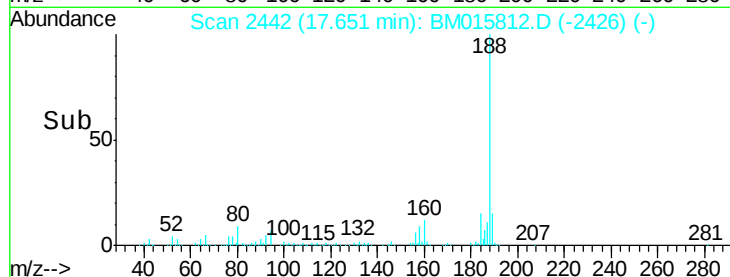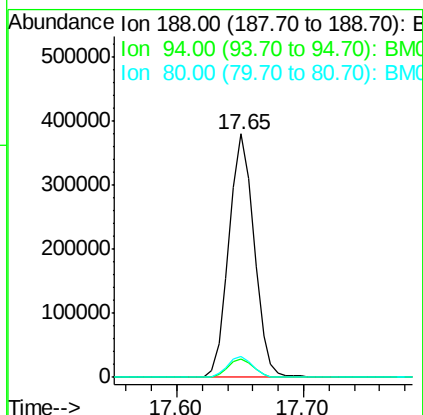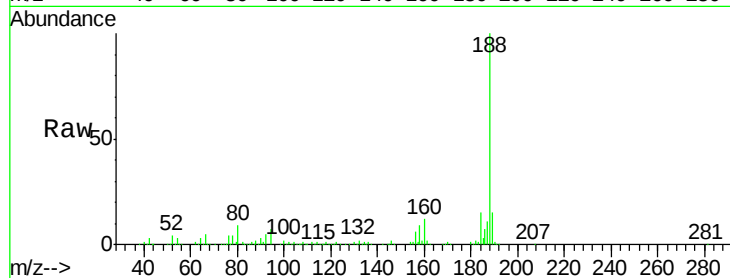

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.76 min Scan# 3140
Delta R.T. -0.01 min
Lab File: BM015812.D
Acq: 06 Jul 2018 21:21

Tgt Ion:240 Resp: 383563
Ion Ratio Lower Upper
240 100
120 10.3 8.2 12.2
236 25.3 20.0 30.0

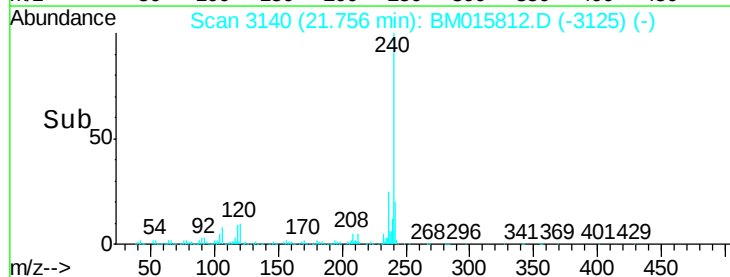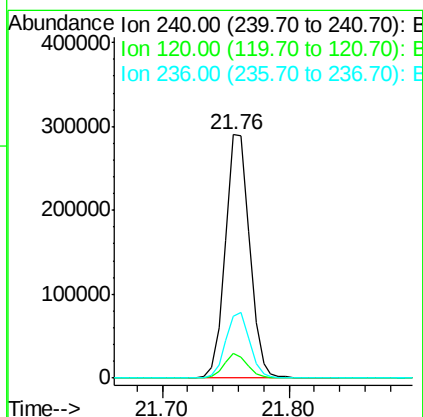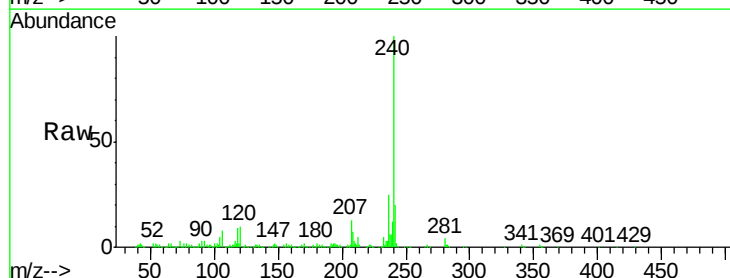

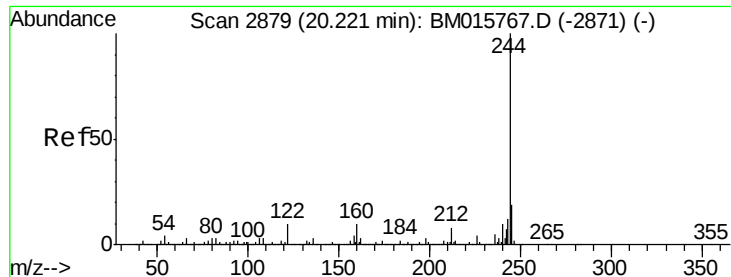

#78

Terphenyl-d14

Concen: Below ng

RT: 20.22 min Scan# 2878

Delta R.T. -0.01 min

Lab File: BM015812.D

Acq: 06 Jul 2018 21:21

Instrument :

BNA_M

ClientSampleId :

GF-02


Tgt Ion:244 Resp: 2718678

Ion Ratio Lower Upper

244 100

212 8.3 4.9 7.3#




122 9.9 6.2 9.4#

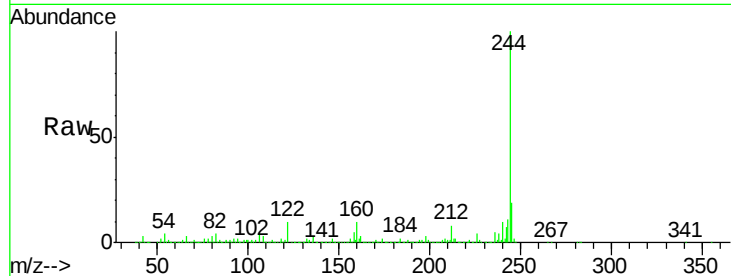

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

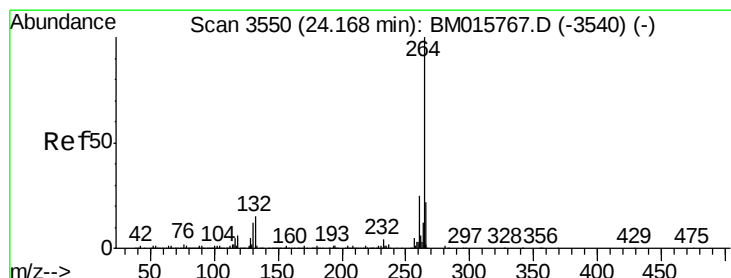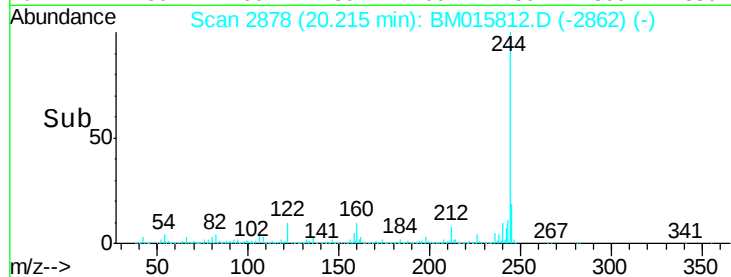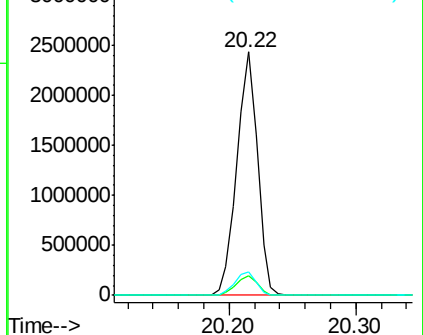

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.16 min Scan# 3549

Delta R.T. -0.01 min

Lab File: BM015812.D

Acq: 06 Jul 2018 21:21


Tgt Ion:264 Resp: 343084

Ion Ratio Lower Upper

264 100

260 24.5 18.6 27.8

265 22.0 17.3 25.9

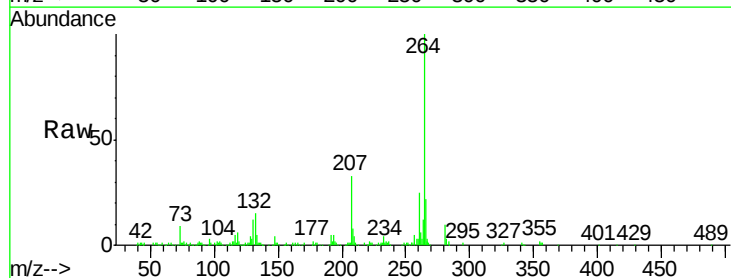

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

