
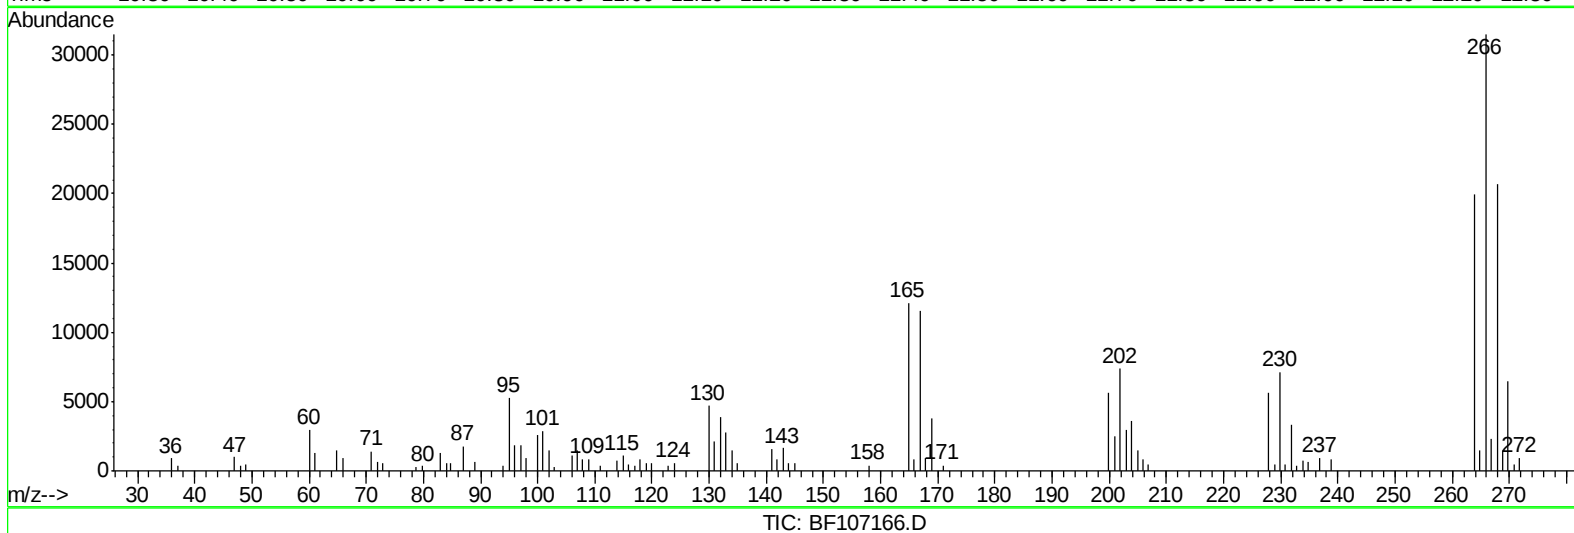


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070618\
Data File : BF107166.D
Acq On : 6 Jul 2018 12:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 07 05:30:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

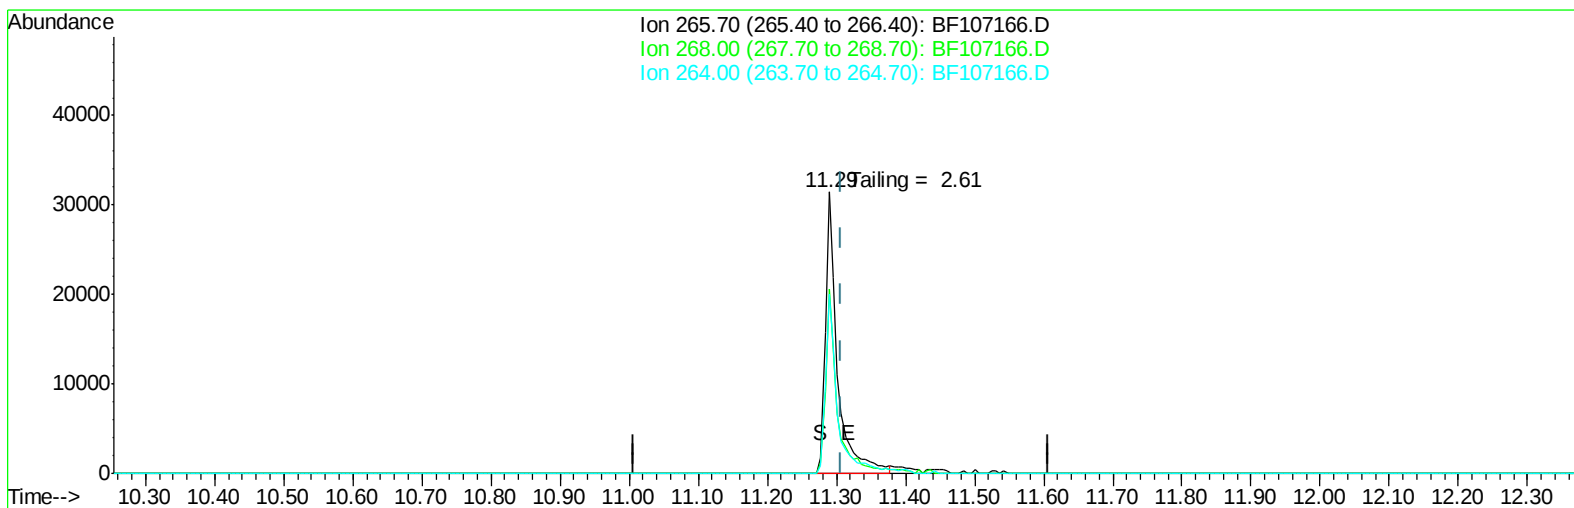

(69) Pentachlorophenol (C)

11.289min (-0.018) 0.00ng




response 37975

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.64
264.00	61.90	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070618\
Data File : BF107166.D
Acq On : 6 Jul 2018 12:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 07 05:30:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

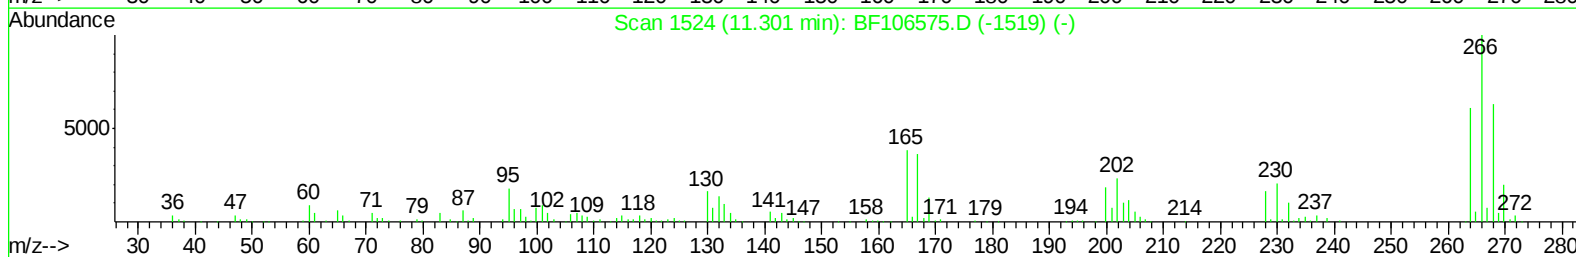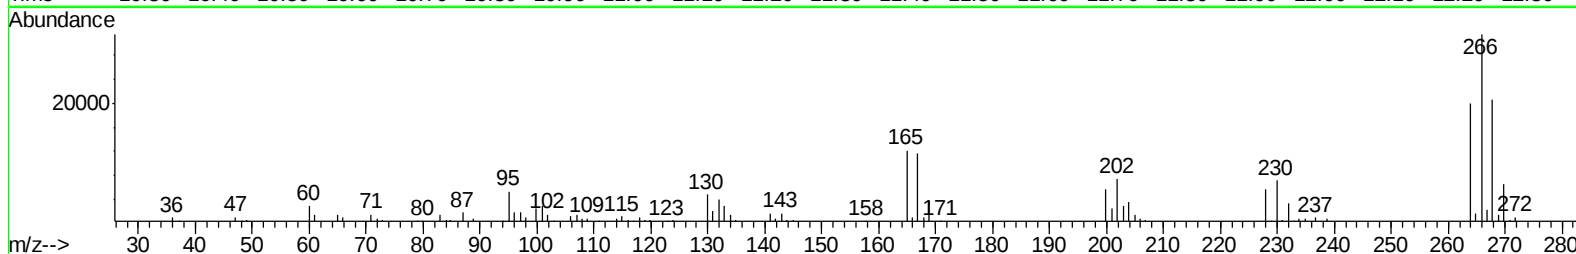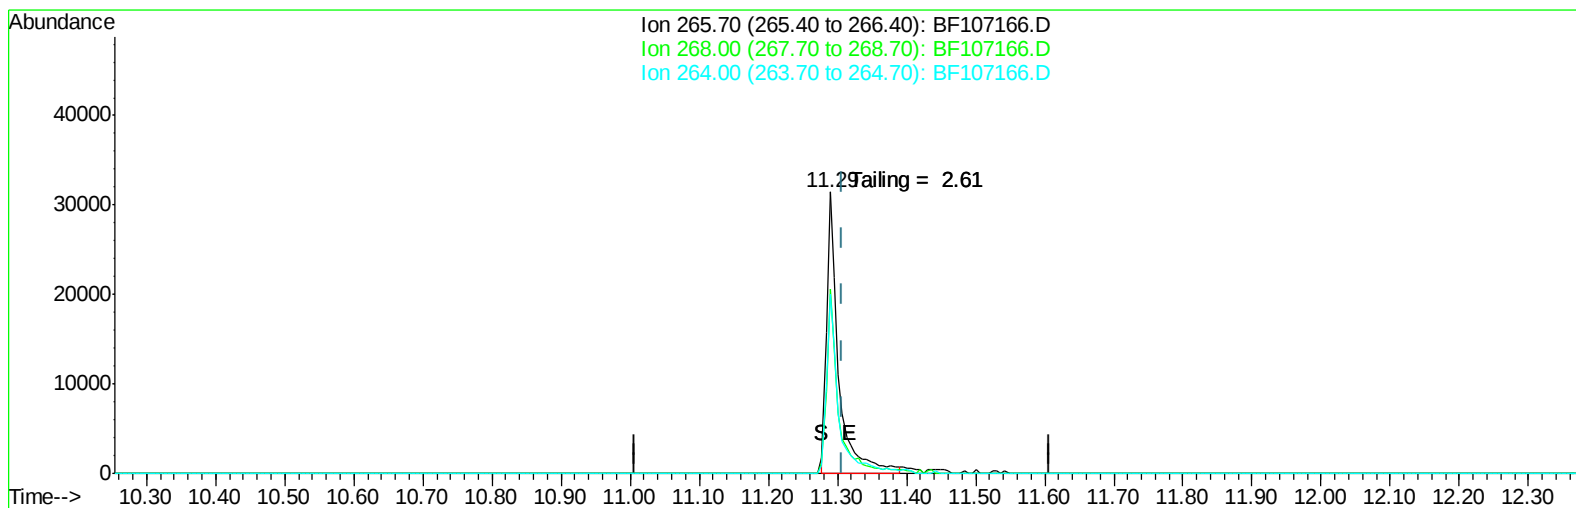

TIC: BF107166.D

(69) Pentachlorophenol (C)

11.289min (-0.018) 0.00ng




response 37975

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.64
264.00	61.90	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070618\
Data File : BF107166.D
Acq On : 6 Jul 2018 12:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 07 05:30:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

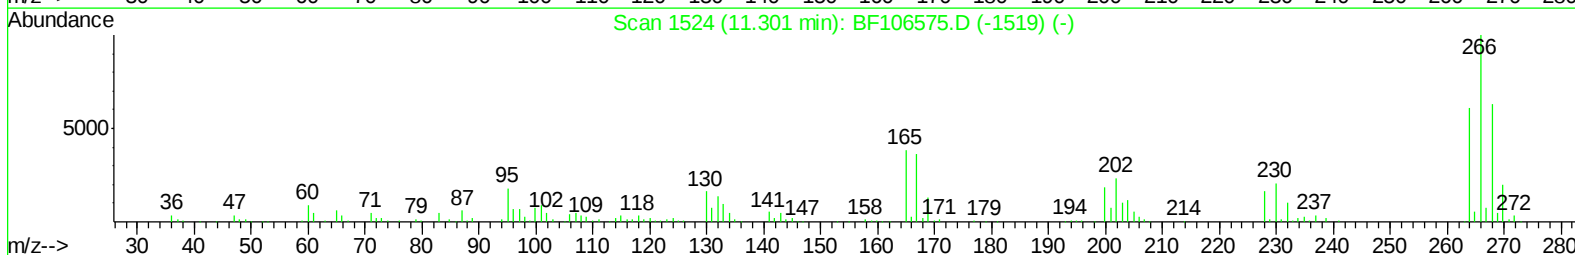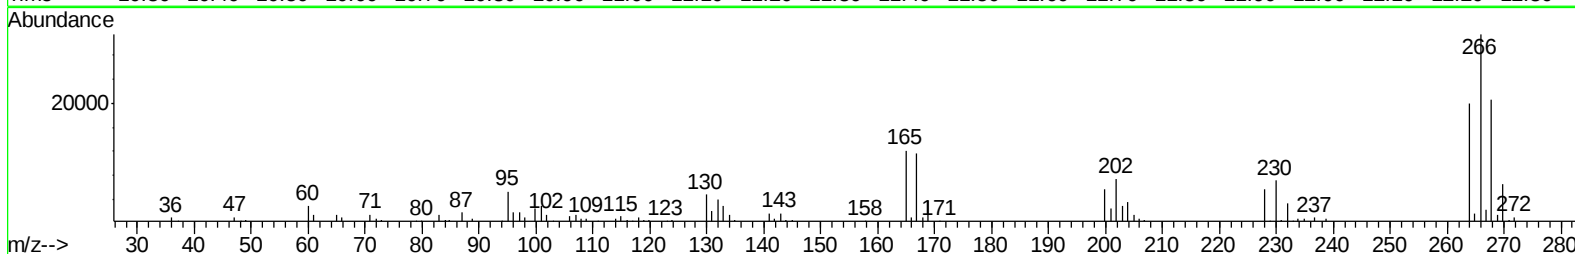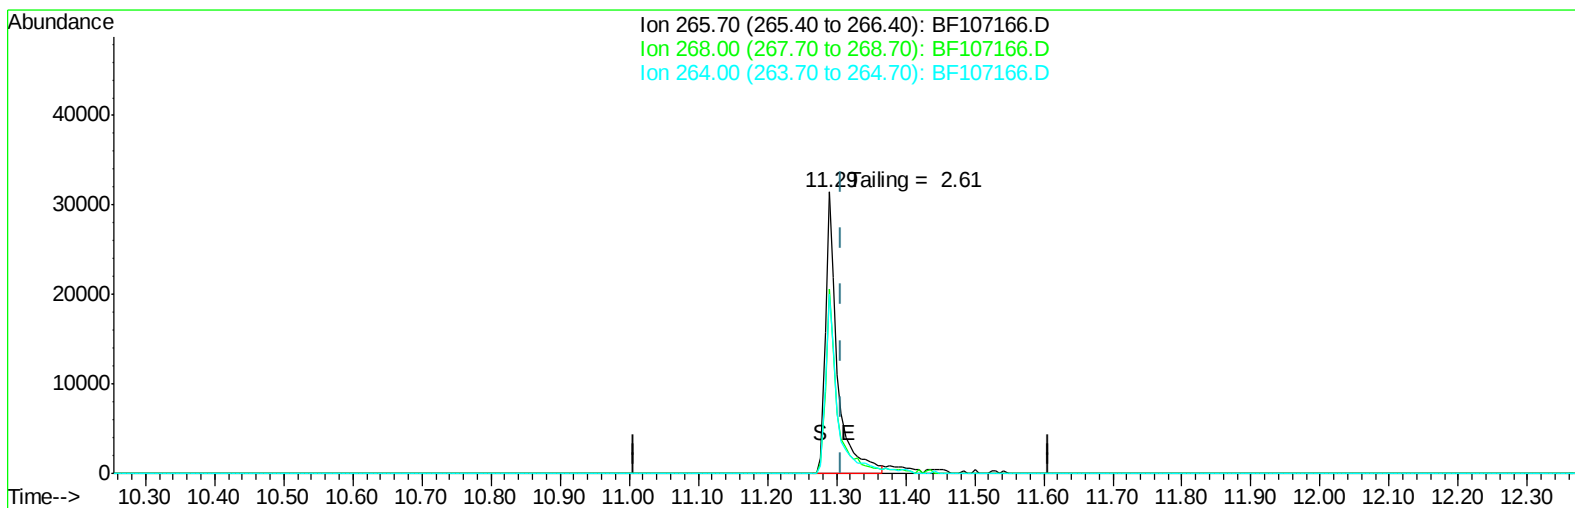

TIC: BF107166.D

(69) Pentachlorophenol (C)

11.289min (-0.018) 0.00ng

response 37975

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.64
264.00	61.90	63.43
0.00	0.00	0.00