

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070618\
 Data File : BM015807.D
 Acq On : 06 Jul 2018 18:17
 Operator : SJ/JU
 Sample : PB110790BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB110790BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.810	421	429	463	rBV	3142759	4552604	26.50%	5.709%
2	7.463	701	710	744	rBV	2973974	4837140	28.16%	6.065%
3	7.834	765	773	793	rBV	3171330	5107882	29.73%	6.405%
4	8.304	845	853	872	rVB	531649	869548	5.06%	1.090%
5	8.633	899	909	926	rBV	2249453	3741065	21.78%	4.691%
6	9.492	1047	1055	1087	rBV	1727328	2939162	17.11%	3.685%
7	11.133	1325	1334	1351	rBV	639247	1066365	6.21%	1.337%
8	13.551	1737	1745	1769	rBV	4256415	6169793	35.91%	7.736%
9	14.927	1971	1979	1996	rBV2	820494	1258770	7.33%	1.578%
10	16.404	2222	2230	2266	rBV	3188960	4375304	25.47%	5.486%
11	17.651	2436	2442	2454	rBV	921333	1282775	7.47%	1.608%
12	20.156	2608	2868	2871	rBV9	22905	771151	4.49%	0.967%
13	20.215	2871	2878	3135	rBV3	5362413	10365901	60.34%	12.998%
14	21.762	3135	3141	3543	rVV3	772104	15233204	88.67%	19.101%
15	24.162	3543	3549	4437	rVV	443001	17180224	100.00%	21.542%


Sum of corrected areas: 79750888

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070618\
Data File : BM015807.D
Acq On : 06 Jul 2018 18:17
Operator : SJ/JU
Sample : PB110790BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB110790BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: RTEINT.P

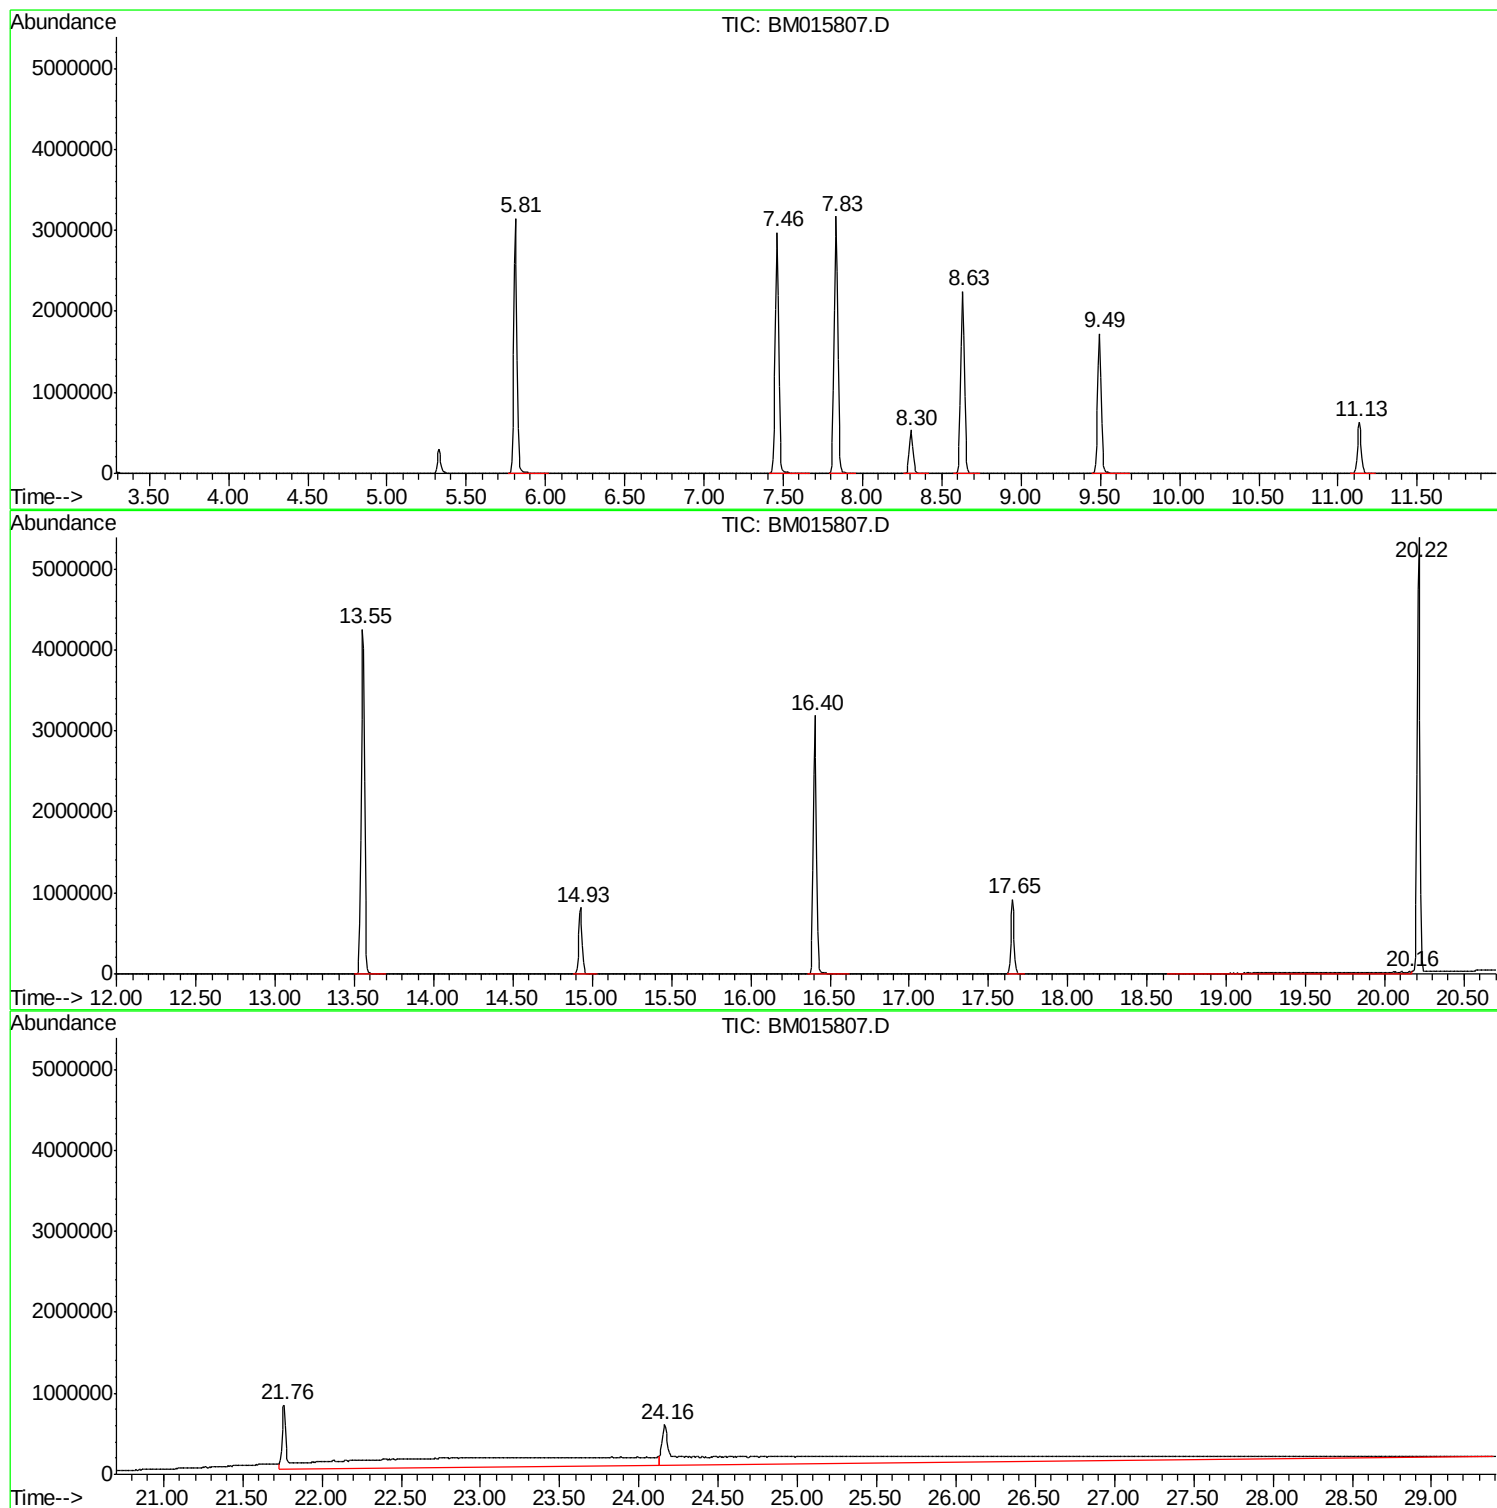

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070618\
Data File : BM015807.D
Acq On : 06 Jul 2018 18:17
Operator : SJ/JU
Sample : PB110790BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB110790BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: RTEINT.P

Peak Number 1 unknown7.83 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.83	117.48 ng	5107880	1,4-Dichlorobenzene-d4	8.30

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	25
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	22
5		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	22

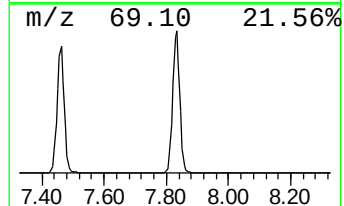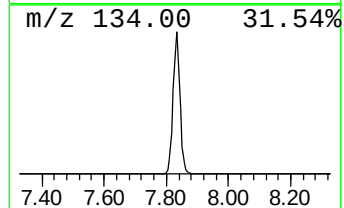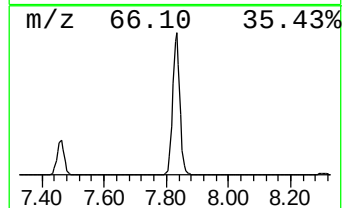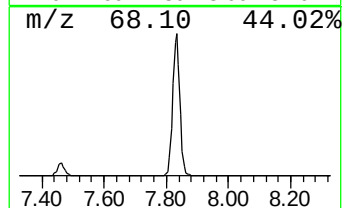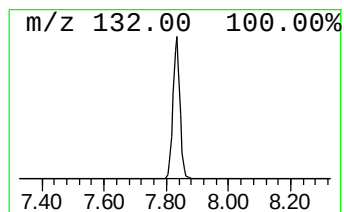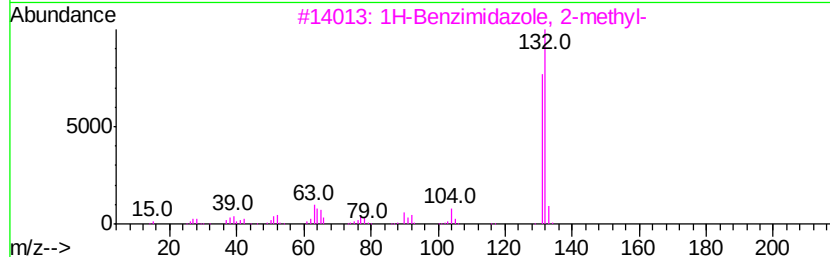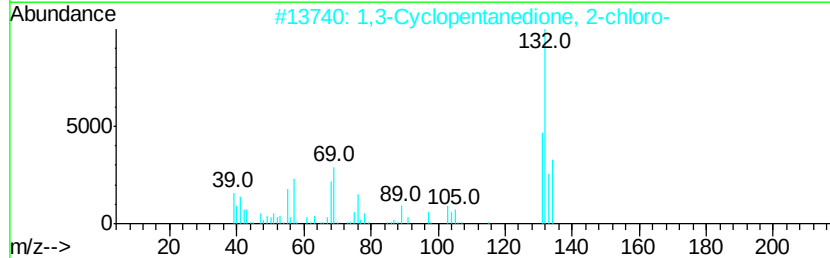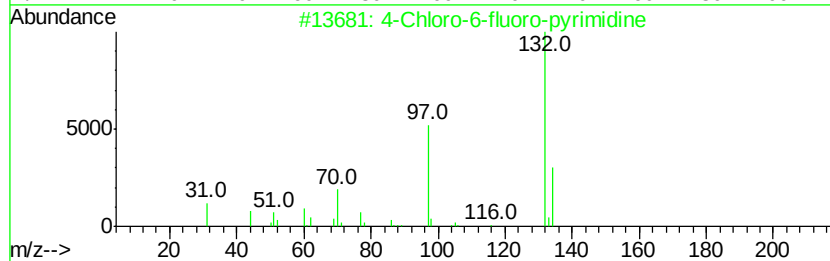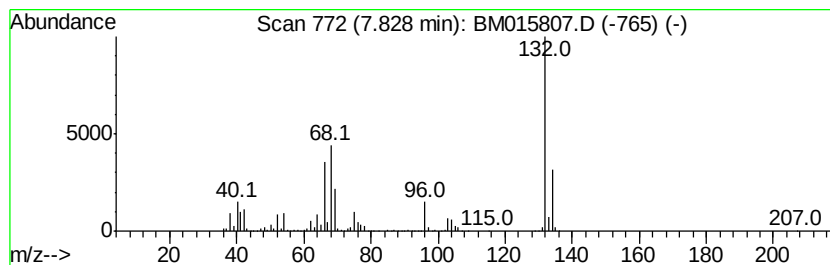

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070618\
Data File : BM015807.D
Acq On : 06 Jul 2018 18:17
Operator : SJ/JU
Sample : PB110790BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB110790BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.83	7.83	117.5	ng	5107880	1	8.30	869548	20.0