


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070618\
 Data File : BM015803.D
 Acq On : 06 Jul 2018 15:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 05 17:39:50 2018

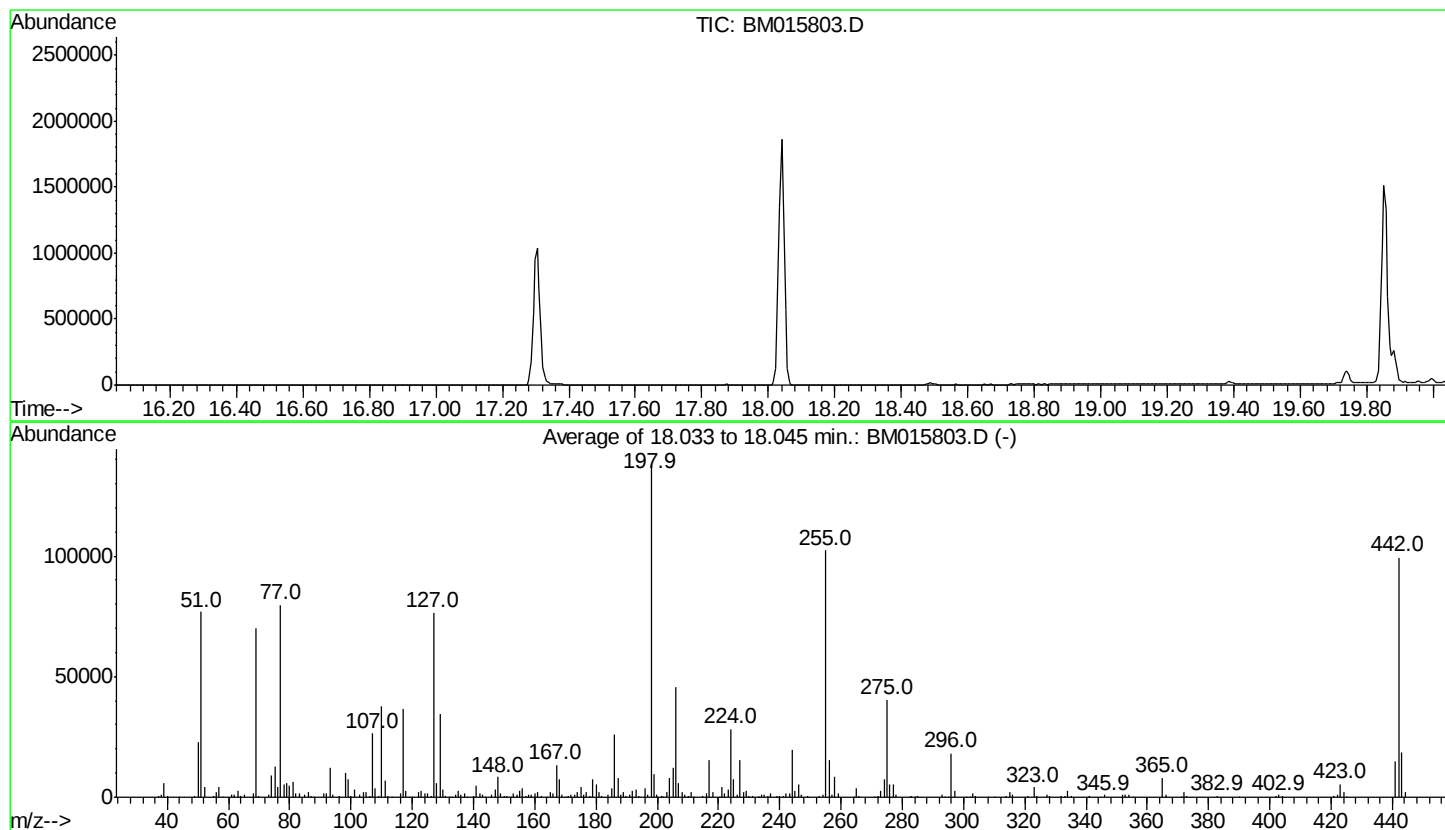

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.9	76800	PASS
68	69	0.00	2	1.9	1355	PASS
69	198	0.00	100	50.9	69965	PASS
70	69	0.00	2	0.5	318	PASS
127	198	10	80	55.7	76613	PASS
197	198	0.00	2	0.7	921	PASS
198	198	100	100	100.0	137474	PASS
199	198	5	9	6.9	9505	PASS
275	198	10	60	29.3	40346	PASS
365	198	1	100	5.8	7999	PASS
441	443	0.01	100	81.3	15072	PASS
442	198	50	100	72.3	99346	PASS
443	442	15	24	18.7	18548	PASS